

6A

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Instrument ID: E Calibration Date(s): 04/01/05 04/01/05

Heated Purge: (Y/N) Y Calibration Times: 9:32 11:48

GC Column: RTX-624 ID: 0.32 (mm)

LAB FILE ID:		vstd010	<u>E2604.D</u>	vstd020	<u>E2605.D</u>		
vstd050	<u>E2606.D</u>	vstd100	<u>E2607.D</u>	vstd200	<u>E2608.D</u>		
COMPOUND	vstd010	vstd020	vstd050	vstd100	vstd200	RRF	% RSD
4-Bromofluorobenzene	0.479	0.475	0.479	0.496	0.485	0.483	0.0
Dibromofluoromethane	0.672	0.673	0.662	0.696	0.698	0.680	0.0
Toluene-d8	1.155	1.165	1.178	1.170	1.195	1.172	0.0

* Compounds with required minimum RRF and maximum %RSD values.
All other compounds must meet a minimum RRF of 0.010.

Response Factor Report inst e

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

Calibration Files

10 =E2604.D 20 =E2605.D 50 =E2606.D
 100 =E2607.D 200 =E2608.D 5.0 =E2603.D

Compound	10	20	50	100	200	5.0	Avg	%RSD
-----ISTD-----								
1) I pentafluorobenzene								
2) T dichlorodifluoromet	0.672	0.673	0.662	0.696	0.698	0.704	0.684	2.50
3) P chloromethane	1.310	1.274	1.260	1.281	1.275	1.341	1.290	2.33
4) C vinyl chloride	0.756	0.756	0.759	0.809	0.847	0.761	0.781	4.87
5) T bromomethane	0.411	0.331	0.198	0.164	0.108	0.430	0.274	49.53 <i>0.1193</i>
6) T chloroethane	0.401	0.402	0.397	0.328		0.433	0.392	9.80
7) T trichlorofluorometh	0.740	0.747	0.740	0.769	0.554	0.743	0.716	11.14
8) T Diethyl Ether	0.363	0.343	0.355	0.358	0.360	0.383	0.360	3.66
9) T Acrolein	0.042	0.041	0.041	0.038	0.036	0.046	0.041	8.53
10) T Acetone	0.308	0.258	0.265	0.249	0.262	0.385	0.288	18.05 <i>0.000</i>
11) Iso-propyl alcohol							0.000	1.00
12) CM 1,1-dichloroethene	0.396	0.410	0.419	0.429	0.407	0.407	0.412	2.72
13) T Iodomethane	0.124	0.121	0.138	0.148	0.169	0.117	0.136	14.59
14) T methylene chloride	0.778	0.744	0.753	0.777	0.786	0.848	0.781	4.70
15) T Carbon Disulfide	2.342	2.389	2.468	2.612	2.489	2.240	2.423	5.33
16) T Acrylonitrile	0.198	0.218	0.228	0.237	0.281	0.209	0.228	12.80
17) tert-Butyl alcohol	0.080	0.081	0.087	0.084	0.101	0.091	0.087	9.09
18) T methyl tert-butyl e	1.662	1.674	1.763	1.802	1.887	1.708	1.749	4.91
19) T trans-1,2-dichloroe	0.674	0.674	0.682	0.704	0.667	0.674	0.679	1.91
20) P 1,1-dichloroethane	1.270	1.276	1.304	1.352	1.376	1.262	1.307	3.64
21) T di-isopropyl ether	2.482	2.493	2.609	2.761	2.832	2.462	2.606	6.04
22) T Vinyl Acetate	0.995	1.114	1.173	1.293	1.451	1.056	1.180	14.20
23) ethyl tert-butyl et	1.922	1.942	2.073	2.196	2.341	1.895	2.061	8.62
24) T 2-Butanone	0.397	0.401	0.436	0.416	0.494	0.425	0.428	8.30
25) T 2,2-dichloropropane	0.803	0.794	0.819	0.872	0.911	0.780	0.830	6.12
26) T cis-1,2-dichloroeth	0.757	0.748	0.778	0.810	0.819	0.760	0.779	3.81
27) T bromochloromethane	0.358	0.354	0.370	0.381	0.384	0.369	0.369	3.27
28) C chloroform	1.273	1.276	1.297	1.366	1.376	1.271	1.310	3.70
29) S Dibromofluoromethan	0.622	0.607	0.633	0.632	0.644	0.608	0.624	2.35
30) T Tetrahydrofuran	0.234	0.234	0.239	0.231	0.273	0.310	0.253	12.57
31) T 1,1,1-trichloroetha	0.888	0.897	0.933	0.972	0.987	0.889	0.928	4.69
-----ISTD-----								
32) I 1,4-difluorobenzene								
33) T carbon tetrachlorid	0.553	0.492	0.427	0.426	0.413	0.742	0.509	24.77 <i>0.4145</i>
34) T 1,1-dichloropropene	0.591	0.680	0.598	0.594	0.572	0.601	0.606	6.21
35) M benzene	1.447	1.464	1.491	1.558	1.462	1.474	1.483	2.68
36) T 1,2-dichloroethane	0.528	0.524	0.532	0.529	0.526	0.533	0.529	0.65
37) tert amyl methyl et	0.864	0.871	0.914	0.956	1.004	0.851	0.910	6.59
38) M trichloroethene	0.401	0.409	0.417	0.428	0.421	0.399	0.412	2.84
39) C 1,2-dichloropropane	0.413	0.412	0.422	0.444	0.446	0.405	0.424	4.11
40) T dibromomethane	0.258	0.261	0.271	0.277	0.282	0.257	0.268	3.93
41) T bromodichloromethan	0.516	0.516	0.533	0.558	0.573	0.479	0.529	6.36
42) T 2-Chloroethyl vinyl	0.002	0.002	0.003	0.008		0.479	0.004	74.14 <i>0.4145</i>


Response Factor Report inst e

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

Calibration Files


10 =E2604.D 20 =E2605.D 50 =E2606.D
 100 =E2607.D 200 =E2608.D 5.0 =E2603.D

	Compound	10	20	50	100	200	5.0	Avg	%RSD
43) T	4-Methyl-2-Pentanone	0.453	0.471	0.496	0.493	0.572	0.533	0.503	8.58
44) T	cis-1,3-dichloropro	0.549	0.558	0.607	0.642	0.670	0.493	0.586	11.18
45) S	toluene-d8	1.155	1.165	1.178	1.170	1.195	1.154	1.170	1.30
46) CM	toluene	0.893	0.912	0.917	0.957	0.952	0.915	0.924	2.71
47) T	trans-1,3-dichlorop	0.463	0.487	0.533	0.568	0.612	0.405	0.511	14.65
48) T	1,1,2-trichloroetha	0.308	0.314	0.326	0.331	0.337	0.303	0.320	4.23
49) I	chlorobenzene-d5	-----ISTD-----							
50) T	2-Hexanone	0.311	0.327	0.368	0.386	0.402	0.322	0.353	10.66
51) T	tetrachloroethene	0.384	0.391	0.382	0.399	0.362	0.404	0.387	3.86
52) T	1,3-dichloropropane	0.628	0.640	0.662	0.693	0.688	0.643	0.659	4.09
53) T	dibromochloromethan	0.385	0.391	0.410	0.437	0.434	0.361	0.403	7.35
54) T	1,2-dibromoethane	0.370	0.385	0.399	0.422	0.425	0.375	0.396	5.90
55) PM	chlorobenzene	1.048	1.052	1.052	1.116	1.080	1.099	1.074	2.67
56) T	1,1,1,2-tetrachloro	0.343	0.345	0.348	0.366	0.341	0.334	0.346	3.16
57) C	ethylbenzene	1.789	1.852	1.852	1.990	1.620	1.823	1.821	6.58
58) T	m,p-xylene	0.656	0.673	0.668	0.695	0.642	0.671	0.668	2.65
59) T	o-xylene	0.616	0.650	0.646	0.695	0.654	0.626	0.648	4.24
60) T	styrene	1.060	1.099	1.130	1.222	1.183	1.043	1.123	6.23
61) P	bromoform	0.241	0.243	0.258	0.278	0.285	0.217	0.254	10.08
62) S	4-Bromofluorobenzen	0.479	0.475	0.479	0.496	0.485	0.478	0.482	1.59
63) I	1,4-dichlorobenzene-d	-----ISTD-----							
64) T	isopropylbenzene	3.732	3.913	3.882	4.094	3.546	3.777	3.824	4.85
65) T	bromobenzene	0.911	0.919	0.929	0.960	0.947	0.934	0.933	1.93
66) P	1,1,2,2-tetrachloro	1.156	1.192	1.192	1.197	1.236	1.216	1.198	2.24
67) T	1,2,3-trichloroprop	0.281	0.287	0.291	0.282	0.295	0.293	0.288	1.99
68) T	n-propylbenzene	4.554	4.738	4.699	5.005	3.877	4.553	4.571	8.27
69) T	2-chlorotoluene	2.621	2.716	2.693	2.816	2.736	2.665	2.708	2.46
70) T	4-chlorotoluene	3.064	3.117	3.045	3.180	3.101	3.132	3.107	1.57
71) T	1,3,5-trimethylbenz	2.999	3.129	3.074	3.212	3.038	3.016	3.078	2.61
72) T	tert-butylbenzene	1.842	1.899	1.865	1.934	1.898	1.833	1.878	2.05
73) T	1,2,4-trimethylbenz	2.973	3.056	3.016	3.177	3.013	2.945	3.030	2.69
74) T	sec-butylbenzene	3.852	4.030	4.029	4.287	3.573	3.815	3.931	6.17
75) T	1,3-dichlorobenzene	1.614	1.648	1.631	1.692	1.569	1.669	1.637	2.64
76) T	4-isopropyltoluene	2.942	3.062	3.063	3.224	2.953	2.928	3.029	3.73
77) T	1,4-dichlorobenzene	1.639	1.677	1.639	1.691	1.636	1.712	1.666	1.95
78) T	1,2-dichlorobenzene	1.534	1.614	1.607	1.666	1.610	1.580	1.602	2.71
79) T	n-butylbenzene	2.715	2.834	2.891	3.070	3.032	2.629	2.862	6.05
80) T	1,2-dibromo-3-chlor	0.157	0.164	0.176	0.177	0.207	0.134	0.169	14.37
81) T	1,2,4-trichlorobenz	0.790	0.886	0.891	0.931	0.881	0.769	0.858	7.42
82) T	hexachlorobutadiene	0.416	0.460	0.435	0.455	0.424	0.395	0.431	5.69
83) T	naphthalene	2.049	2.377	2.537	2.588	2.700	1.915	2.361	13.31
84) T	1,2,3-trichlorobenz	0.828	0.908	0.893	0.938	0.878	0.780	0.871	6.61

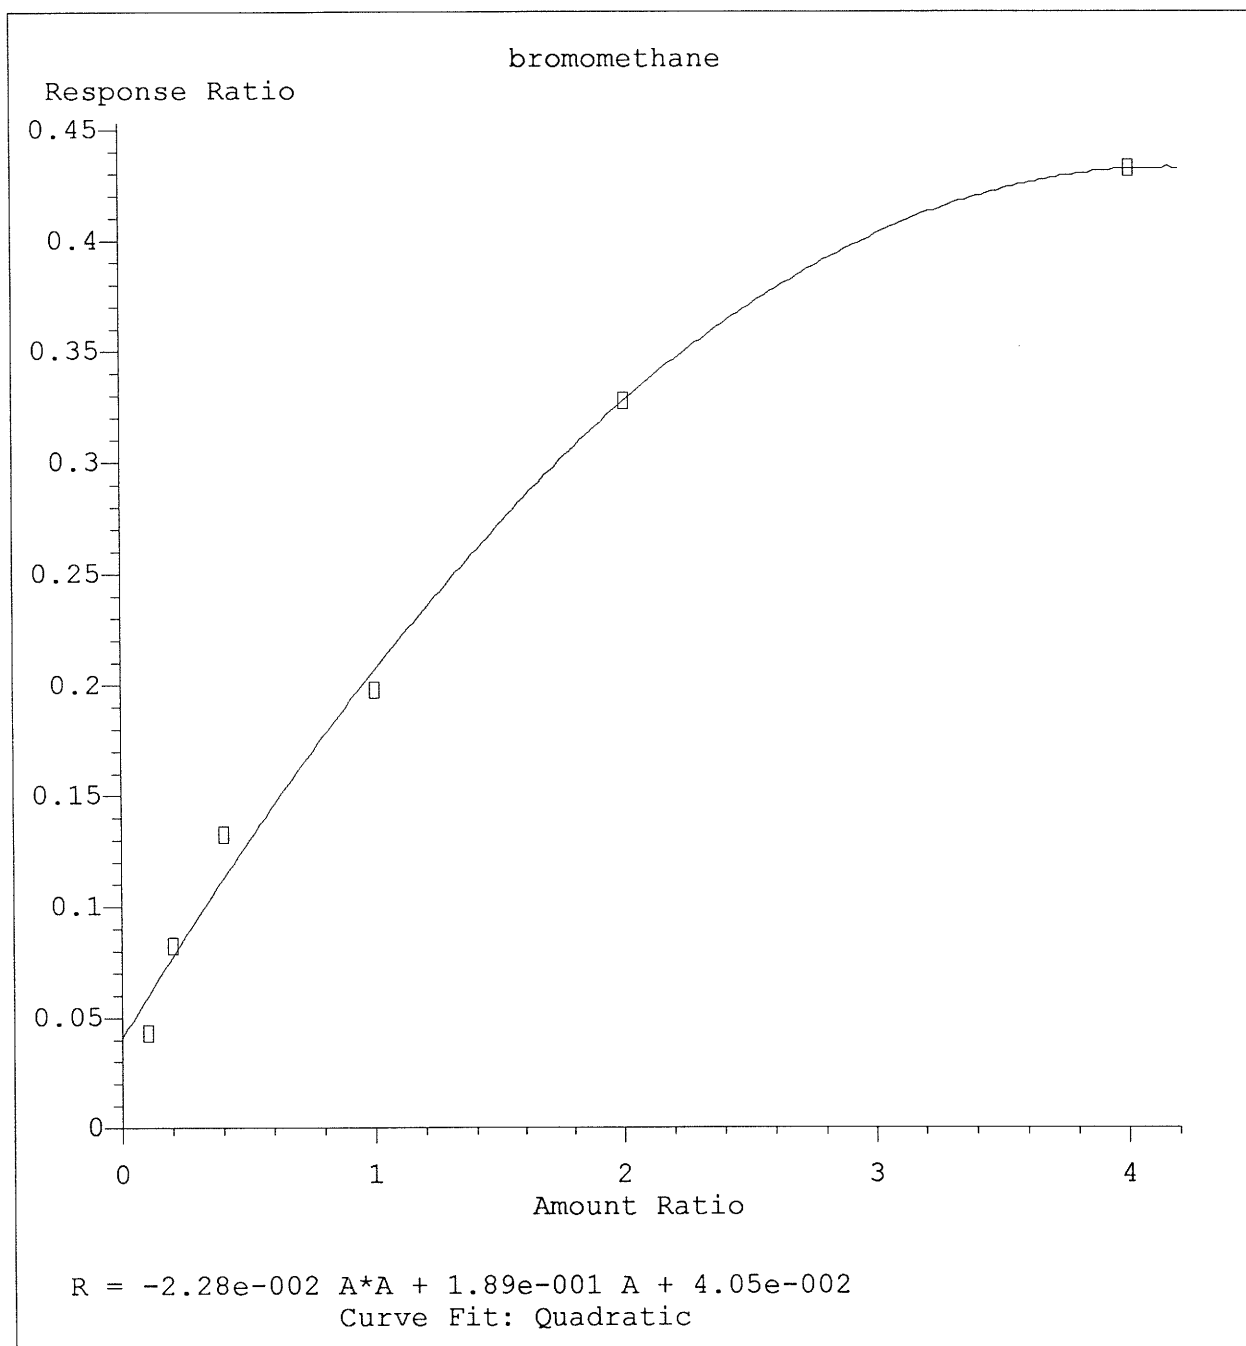


Method Name: C:\HPCHEM\1\DATA\040105\8260ES6.M
Calibration Table Last Updated: Mon Apr 04 10:04:38 2005

000094

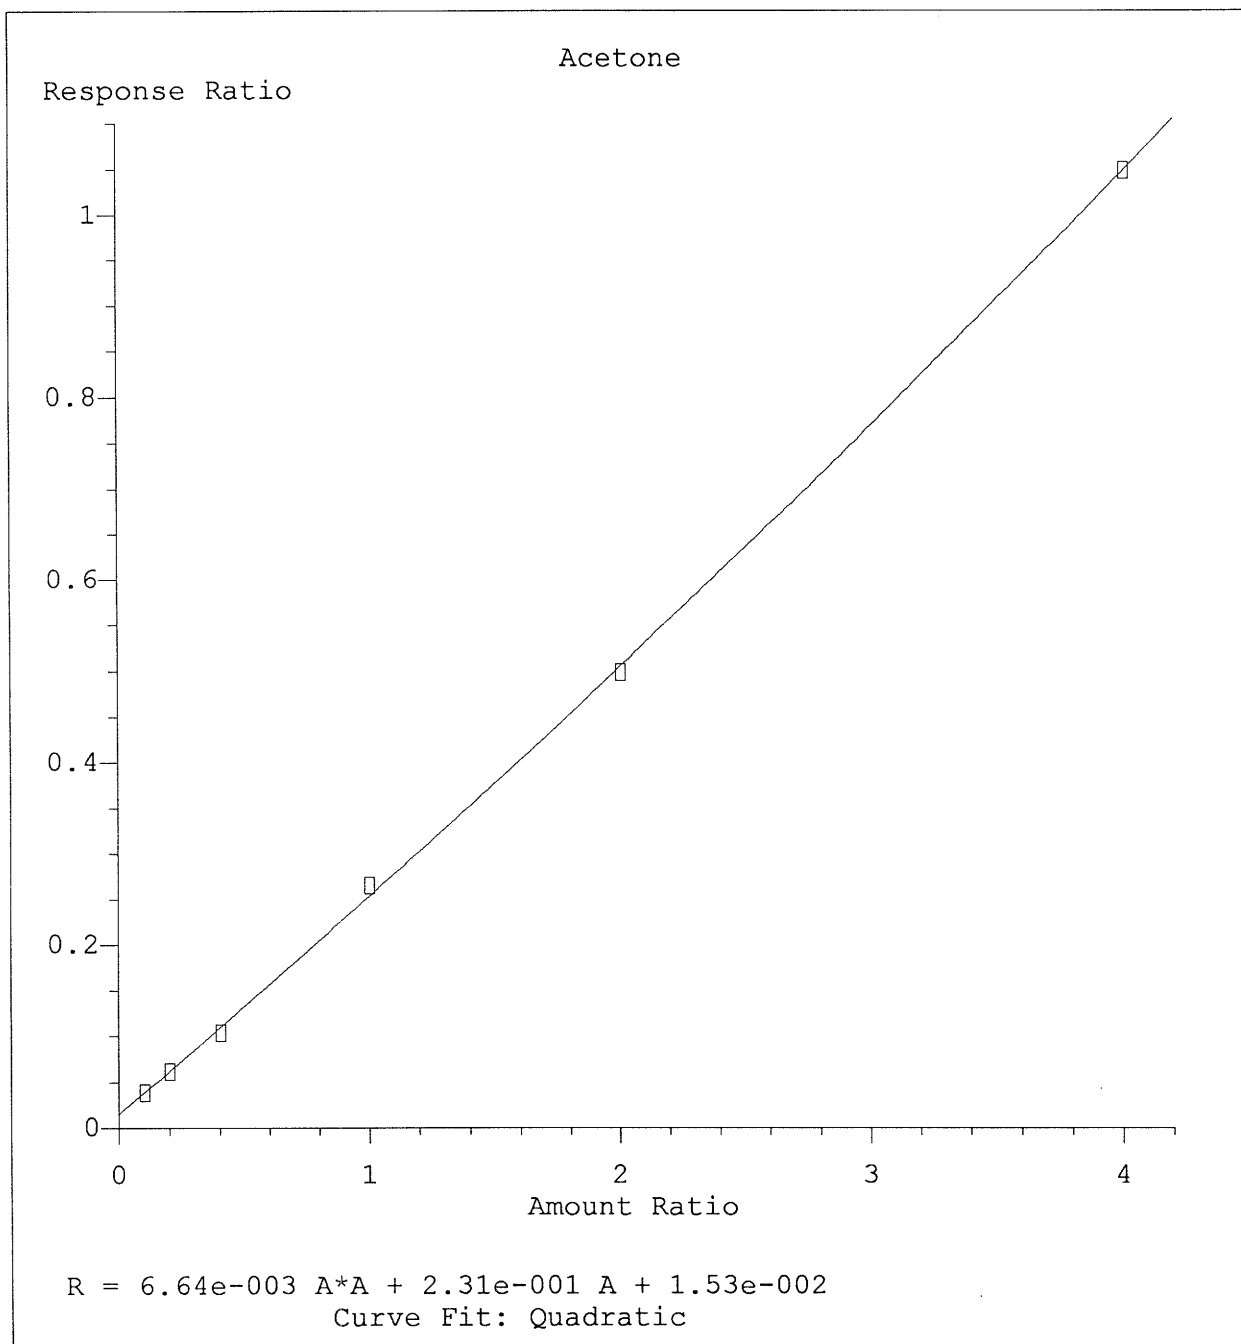


Method Name: C:\HPCHEM\1\DATA\040105\8260ES6.M
Calibration Table Last Updated: Mon Apr 04 10:04:14 2005

000095

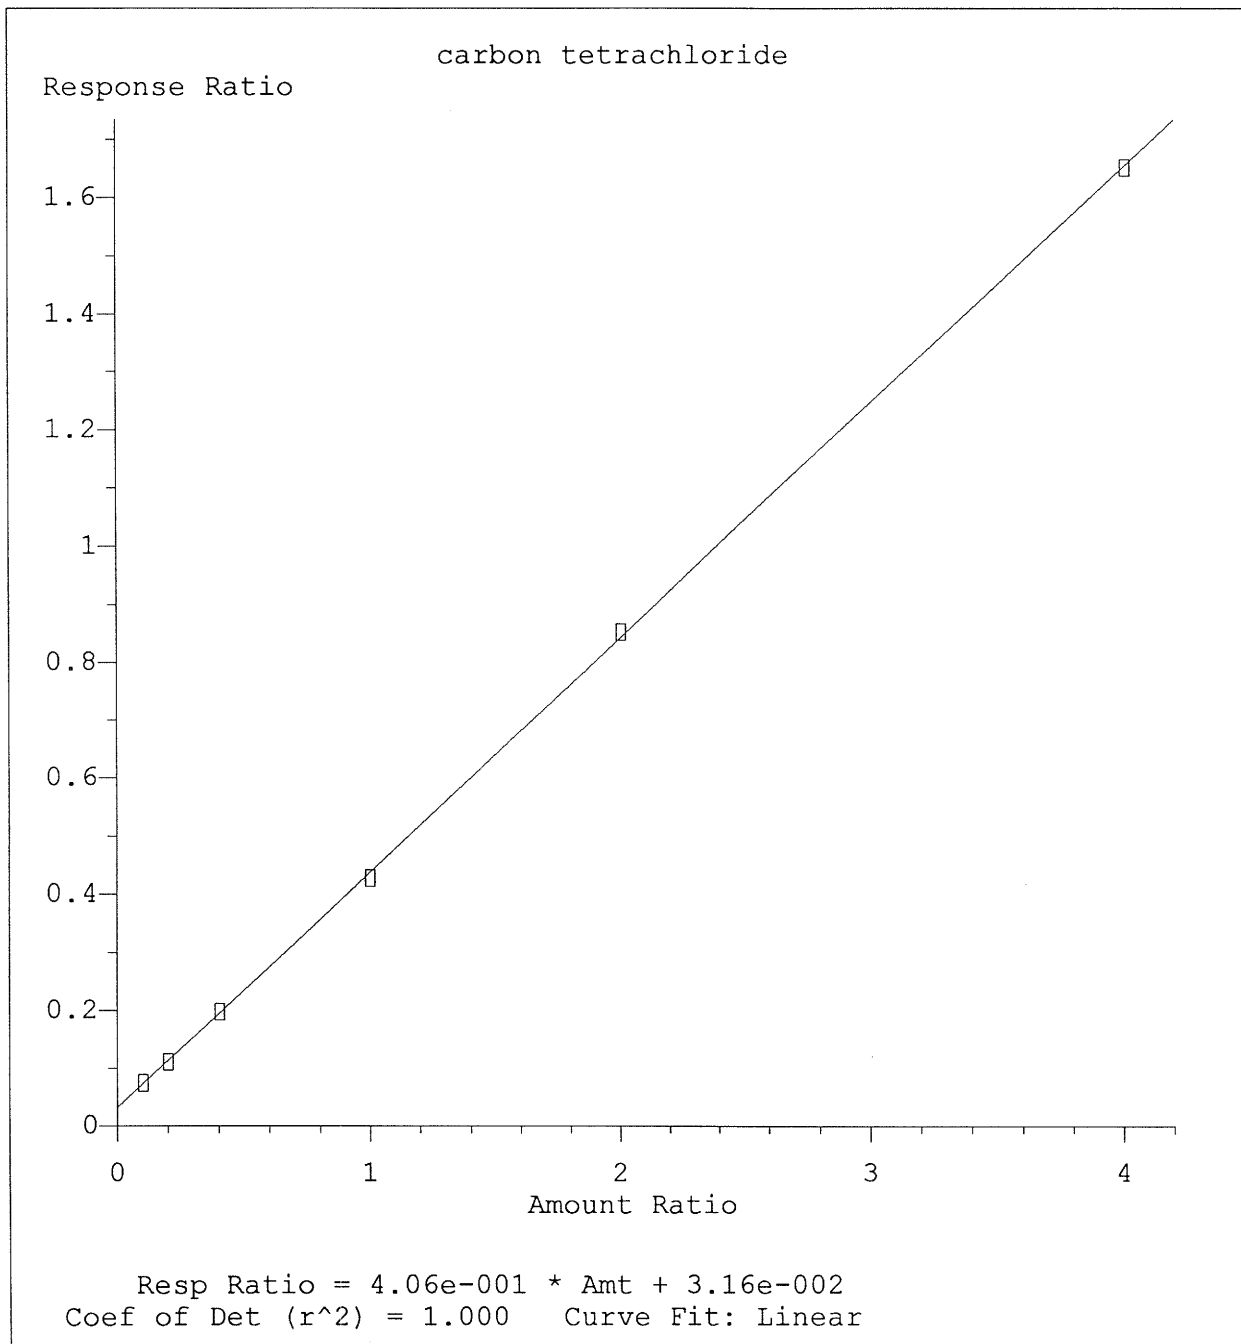

Method Name: C:\HPCHEM\1\DATA\040105\8260ES6.M
Calibration Table Last Updated: Mon Apr 04 10:02:08 2005

000096

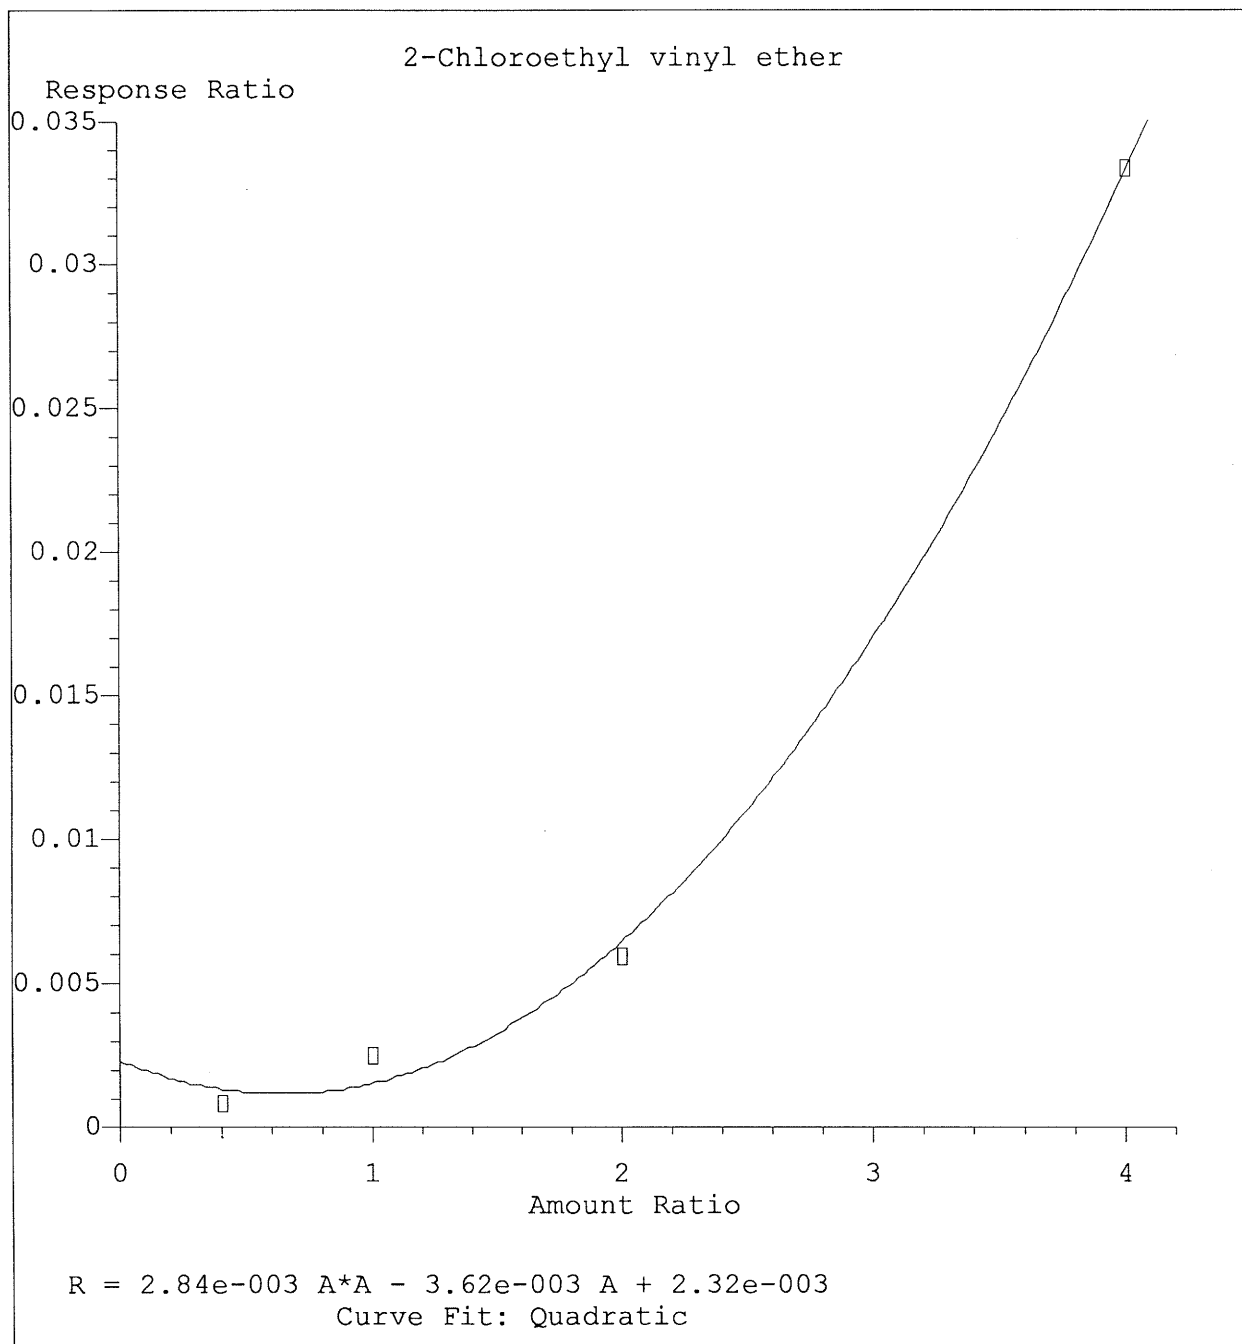

Method Name: C:\HPCHEM\1\DATA\040105\8260ES6.M
Calibration Table Last Updated: Mon Apr 04 10:04:38 2005

000097

Data File : C:\HPCHEM\1\DATA\040105\E2603.D

Vial: 2

Acq On : 1 Apr 05 8:57 am

Operator: xl

Sample : 5ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:29 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.59	168	1916331	50.00	ug/Kg	-0.04
32) 1,4-difluorobenzene	8.78	114	3574388	50.00	ug/Kg	-0.04
49) chlorobenzene-d5	13.93	117	3323328	50.00	ug/Kg	-0.03
63) 1,4-dichlorobenzene-d4	18.43	152	1506165	50.00	ug/Kg	-0.03

System Monitoring Compounds

29) Dibromofluoromethane	7.47	113	1165309	47.20	ug/Kg	-0.04
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.40%
45) toluene-d8	11.26	98	4125559	50.11	ug/Kg	-0.04
Spiked Amount	50.000	Range	81 - 120	Recovery	=	100.22%
62) 4-Bromofluorobenzene	16.19	95	1589204	50.63	ug/Kg	-0.04
Spiked Amount	50.000	Range	74 - 121	Recovery	=	101.26%

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.67	85	134846	6.96	ug/Kg	96
3) chloromethane	1.88	50	256987	5.57	ug/Kg	97
4) vinyl chloride	1.99	62	145823	5.13	ug/Kg	99
5) bromomethane	2.39	96	82362	496.27	ug/Kg	97
6) chloroethane	2.52	64	82946	5.17	ug/Kg	99
7) trichlorofluoromethane	2.81	101	142355	5.17	ug/Kg	100
8) Diethyl Ether	3.23	45	73390	4.84	ug/Kg	89
10) Acetone	3.77	43	73837m	6.32	ug/Kg	96
12) 1,1-dichloroethene	3.54	96	77964	4.38	ug/Kg	94
13) Iodomethane	3.78	142	22347	-13.46	ug/Kg	92
14) methylene chloride	4.44	84	162566	5.16	ug/Kg	95
15) Carbon Disulfide	3.82	76	429205	4.17	ug/Kg	96
16) Acrylonitrile	4.99	53	40022	4.37	ug/Kg	94
17) tert-Butyl alcohol	4.76	59	173970	64.10	ug/Kg	100
18) methyl tert-butyl ether	4.81	73	327331	4.83	ug/Kg	100
19) trans-1,2-dichloroethene	4.81	96	129125	4.61	ug/Kg	96
20) 1,1-dichloroethane	5.60	63	241771	4.45	ug/Kg	99
21) di-isopropyl ether	5.64	45	471777	4.44	ug/Kg	99
22) Vinyl Acetate	5.72	43	202320	4.56	ug/Kg	98
23) ethyl tert-butyl ether	6.26	59	363122	4.51	ug/Kg	97
24) 2-Butanone	6.74	43	81387	4.89	ug/Kg	96
25) 2,2-dichloropropane	6.54	77	149439	4.65	ug/Kg	97
26) cis-1,2-dichloroethene	6.62	96	145667	4.53	ug/Kg	98
27) bromochloromethane	7.03	128	70755	4.65	ug/Kg	94
28) chloroform	7.19	83	243508	4.56	ug/Kg	98
30) Tetrahydrofuran	7.09	42	59451	6.58	ug/Kg	96
31) 1,1,1-trichloroethane	7.37	97	170427	4.57	ug/Kg	99

(#)=qualifier out of range (m)=manual integration

E2603.D 8260ES6.M

Fri Apr 01 19:51:45 2005

000098

Page 1

Data File : C:\HPCHEM\1\DATA\040105\E2603.D

Vial: 2

Acq On : 1 Apr 05 8:57 am

Operator: xl

Sample : 5ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:29 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) carbon tetrachloride	7.58	117	265385m	2.78	ug/Kg	60
34) 1,1-dichloropropene	7.65	75	214789	4.69	ug/Kg	99
35) benzene	7.98	78	526762	4.60	ug/Kg	100
36) 1,2-dichloroethane	8.18	62	190572	4.97	ug/Kg	99
37) tert amyl methyl ether	8.20	73	304307	4.93	ug/Kg	100
38) trichloroethene	9.15	95	142532	4.66	ug/Kg	92
39) 1,2-dichloropropane	9.60	63	144733	4.71	ug/Kg	99
40) dibromomethane	9.81	93	91742	4.82	ug/Kg	96
41) bromodichloromethane	10.12	83	171287	4.67	ug/Kg	99
42) 2-Chloroethyl vinyl ether	11.38	63	47800m	137.63	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.21	43	190391m	5.46	ug/Kg	79
44) cis-1,3-dichloropropene	10.91	75	176313	4.27	ug/Kg	100
46) toluene	11.38	92	327081	4.79	ug/Kg	100
47) trans-1,3-dichloropropene	11.98	75	144860	7.88	ug/Kg	97
48) 1,1,2-trichloroethane	12.28	83	108412	4.82	ug/Kg	93
50) 2-Hexanone	12.74	43	106860m	6.70	ug/Kg	97
51) tetrachloroethene	12.31	166	134126	4.89	ug/Kg	96
52) 1,3-dichloropropane	12.57	76	213586	4.68	ug/Kg	100
53) dibromochloromethane	12.92	129	119892	4.52	ug/Kg	97
54) 1,2-dibromoethane	13.12	107	124709	4.69	ug/Kg	97
55) chlorobenzene	13.98	112	365383	4.81	ug/Kg	91
56) 1,1,1,2-tetrachloroethane	14.17	131	110957	4.73	ug/Kg	97
57) ethylbenzene	14.15	91	605784	4.68	ug/Kg	100
58) m,p-xylene	14.38	106	445935	9.41	ug/Kg	95
59) o-xylene	15.12	106	208155	4.51	ug/Kg	99
60) styrene	15.18	104	346578	4.43	ug/Kg	98
61) bromoform	15.57	173	71994	4.46	ug/Kg	99
64) isopropylbenzene	15.81	105	568919	4.48	ug/Kg	99
65) bromobenzene	16.43	156	140636	4.66	ug/Kg	93
66) 1,1,2,2-tetrachloroethane	16.59	83	183144	5.06	ug/Kg	99
67) 1,2,3-trichloropropane	16.64	110	44161	4.98	ug/Kg	94
68) n-propylbenzene	16.60	91	685735	4.52	ug/Kg	98
69) 2-chlorotoluene	16.81	91	401346	4.34	ug/Kg	94
70) 4-chlorotoluene	17.03	91	471778	4.71	ug/Kg	97
71) 1,3,5-trimethylbenzene	16.97	105	454301	4.53	ug/Kg	98
72) tert-butylbenzene	17.56	91	276093	4.51	ug/Kg	94
73) 1,2,4-trimethylbenzene	17.69	105	443560	4.48	ug/Kg	100
74) sec-butylbenzene	18.00	105	574556	4.41	ug/Kg	98
75) 1,3-dichlorobenzene	18.27	146	251345	4.66	ug/Kg	99
76) 4-isopropyltoluene	18.29	119	440983	4.47	ug/Kg	99
77) 1,4-dichlorobenzene	18.47	146	257927	4.76	ug/Kg	96

(#)=qualifier out of range (m)=manual integration

E2603.D 8260ES6.M

Fri Apr 01 19:51:45 2005

000099

Page 2

Data File : C:\HPCHEM\1\DATA\040105\E2603.D

Vial: 2

Acq On : 1 Apr 05 8:57 am

Operator: xl

Sample : 5ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:29 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
78) 1,2-dichlorobenzene	19.24	146	237996	4.56 ug/Kg	97
79) n-butylbenzene	19.13	91	395945	4.23 ug/Kg	98
80) 1,2-dibromo-3-chloropropan	21.17	75	20175	7.47 ug/Kg	96
81) 1,2,4-trichlorobenzene	23.03	180	115787	4.22 ug/Kg	98
82) hexachlorobutadiene	23.32	225	59471	4.34 ug/Kg	99
83) naphthalene	23.56	128	288427	4.15 ug/Kg	100
84) 1,2,3-trichlorobenzene	24.11	180	117512	4.34 ug/Kg	100


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2603.D
 Acq On : 1 Apr 05 8:57 am
 Sample : 5ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 19:29 19105

Vial: 2
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

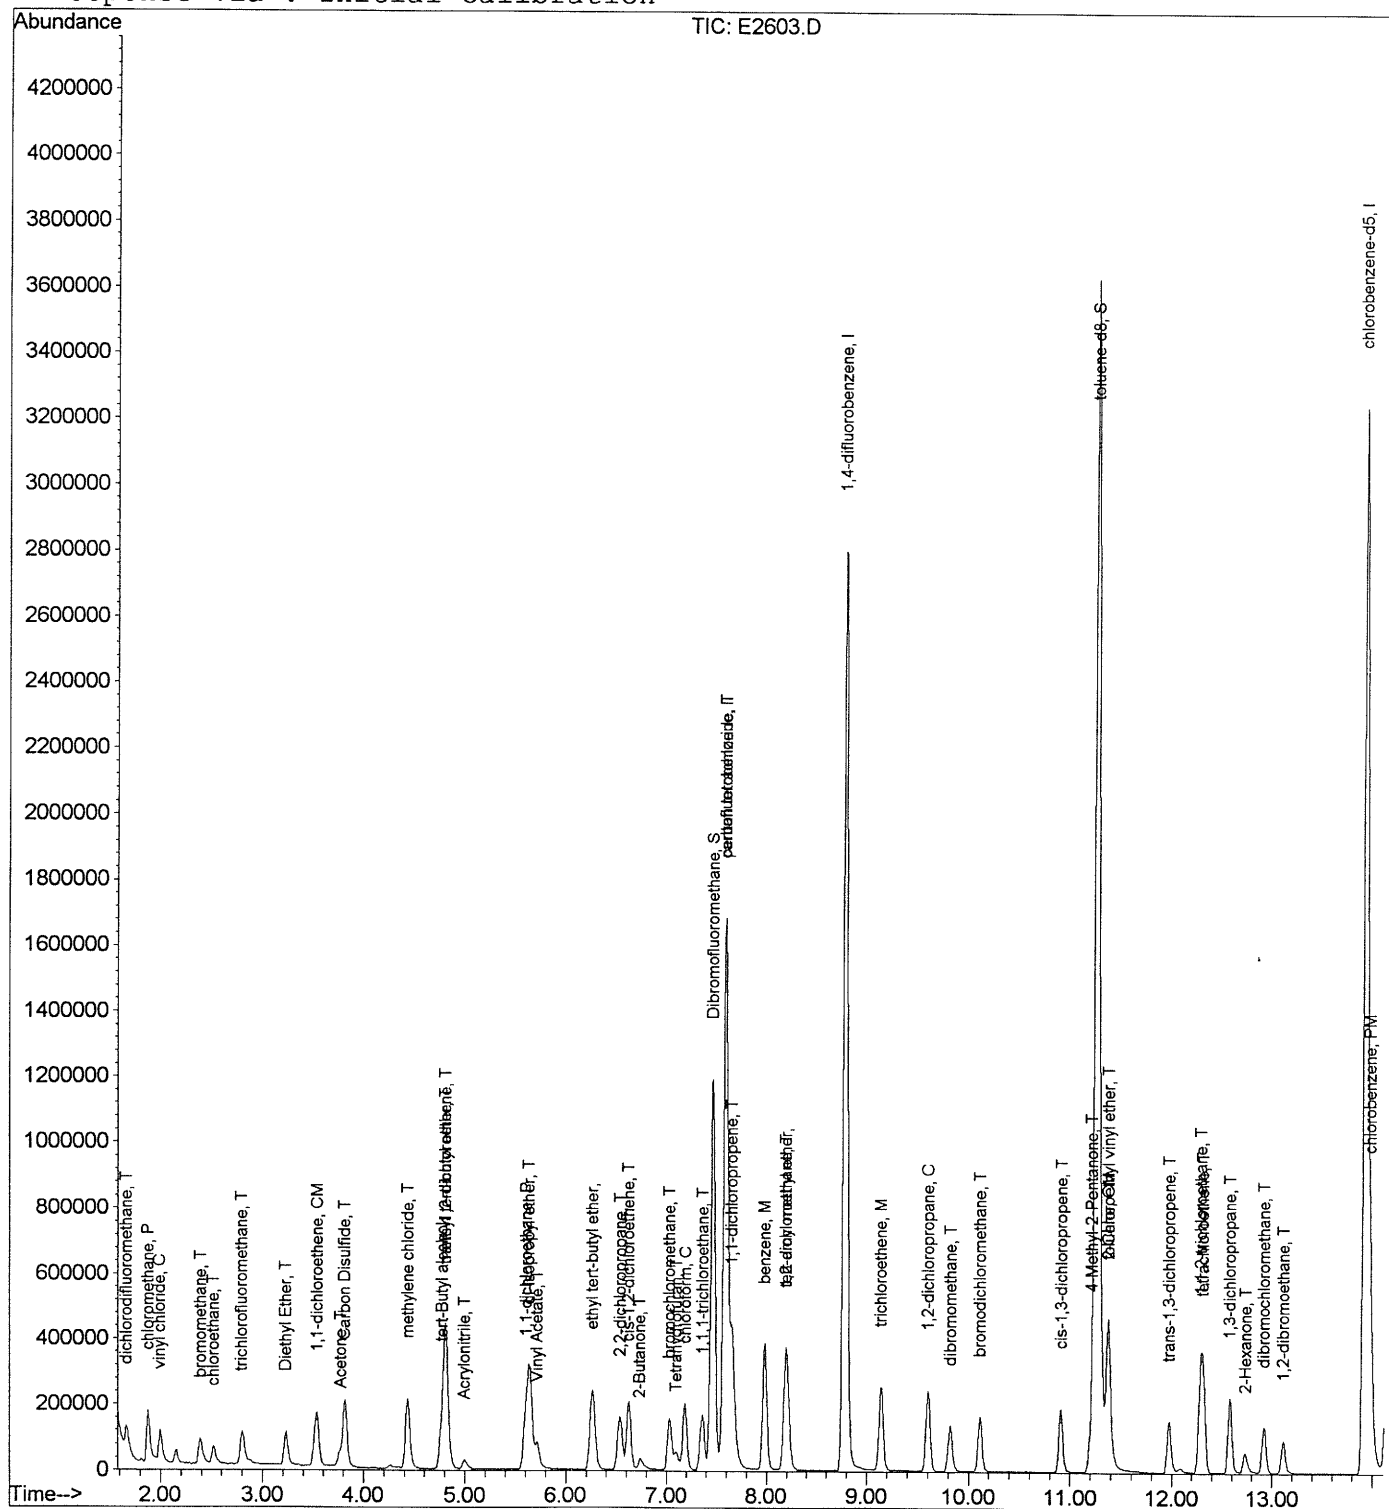


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2603.D
 Acq On : 1 Apr 05 8:57 am
 Sample : 5ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 19:29 19105

Vial: 2
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

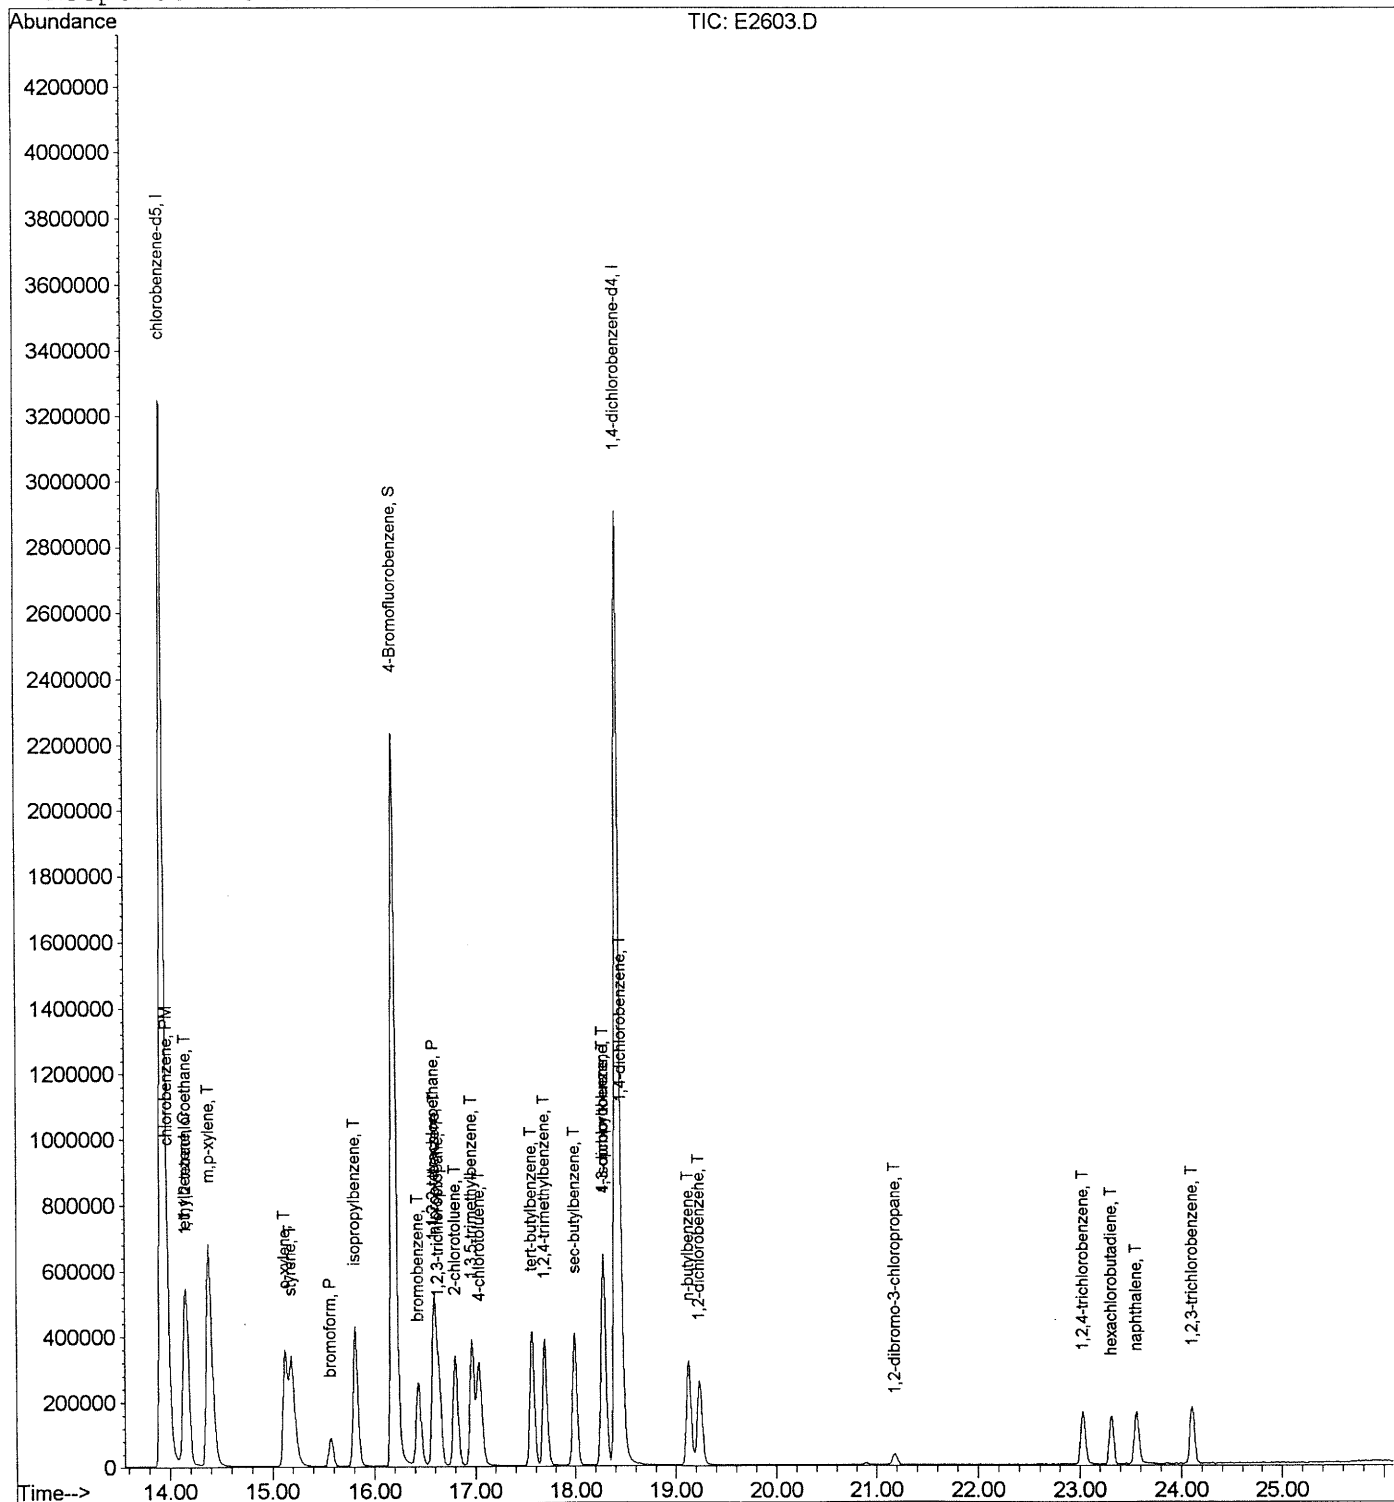

Data File : C:\HPCHEM\1\DATA\040105\E2604.D

Vial: 3

Acq On : 1 Apr 05 9:32 am

Operator: xl

Sample : 10ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:27 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.60	168	1906126	50.00	ug/Kg	-0.03
32) 1,4-difluorobenzene	8.79	114	3533472	50.00	ug/Kg	-0.03
49) chlorobenzene-d5	13.93	117	3351270	50.00	ug/Kg	-0.03
63) 1,4-dichlorobenzene-d4	18.42	152	1524662	50.00	ug/Kg	-0.03

System Monitoring Compounds

29) Dibromofluoromethane	7.47	113	1184761	48.24	ug/Kg	-0.03
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.48%		
45) toluene-d8	11.26	98	4082477	50.16	ug/Kg	-0.03
Spiked Amount 50.000	Range 81 - 120		Recovery =	100.32%		
62) 4-Bromofluorobenzene	16.20	95	1604709	50.70	ug/Kg	-0.03
Spiked Amount 50.000	Range 74 - 121		Recovery =	101.40%		

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.67	85	256270	13.29	ug/Kg	98
3) chloromethane	1.88	50	499566	10.88	ug/Kg	97
4) vinyl chloride	2.00	62	288039	10.19	ug/Kg	99
5) bromomethane	2.39	96	156751	7.49	ug/Kg	94
6) chloroethane	2.52	64	152846	9.57	ug/Kg	99
7) trichlorofluoromethane	2.80	101	282238	10.31	ug/Kg	100
8) Diethyl Ether	3.23	45	138255	9.17	ug/Kg	91
9) Acrolein	4.80	56	79271	44.55	ug/Kg	97
10) Acetone	3.77	43	117583	10.12	ug/Kg	97
12) 1,1-dichloroethene	3.55	96	151094	8.54	ug/Kg	99
14) methylene chloride	4.45	84	296611	9.46	ug/Kg	97
15) Carbon Disulfide	3.83	76	892862	8.72	ug/Kg	97
16) Acrylonitrile	5.00	53	75300	8.27	ug/Kg	96
17) tert-Butyl alcohol	4.77	59	303385	106.10	ug/Kg	100
18) methyl tert-butyl ether	4.82	73	633508	9.40	ug/Kg	100
19) trans-1,2-dichloroethene	4.81	96	257068	9.23	ug/Kg	97
20) 1,1-dichloroethane	5.61	63	483991	8.96	ug/Kg	97
21) di-isopropyl ether	5.65	45	946290	8.95	ug/Kg	100
22) Vinyl Acetate	5.73	43	379161	8.59	ug/Kg	99
23) ethyl tert-butyl ether	6.27	59	732833	9.15	ug/Kg	99
24) 2-Butanone	6.74	43	151276	9.15	ug/Kg	99
25) 2,2-dichloropropane	6.54	77	306143	9.57	ug/Kg	97
26) cis-1,2-dichloroethene	6.63	96	288432	9.03	ug/Kg	99
27) bromochloromethane	7.03	128	136534	9.03	ug/Kg	97
28) chloroform	7.19	83	485440	9.13	ug/Kg	98
30) Tetrahydrofuran	7.10	42	89371	9.94	ug/Kg	96
31) 1,1,1-trichloroethane	7.37	97	338617	9.14	ug/Kg	99

(#)= qualifier out of range (m) = manual integration

E2604.D 8260ES6.M

Fri Apr 01 19:51:59 2005

xl 4/1/05

000103

Data File : C:\HPCHEM\1\DATA\040105\E2604.D

Vial: 3

Acq On : 1 Apr 05 9:32 am

Operator: xl

Sample : 10ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:27 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) carbon tetrachloride	7.59	117	390776m	7.32	ug/Kg	77
34) 1,1-dichloropropene	7.66	75	417684	9.23	ug/Kg	99
35) benzene	7.99	78	1022805	9.04	ug/Kg	99
36) 1,2-dichloroethane	8.18	62	373316	9.84	ug/Kg	98
37) tert amyl methyl ether	8.21	73	610782	10.02	ug/Kg	100
38) trichloroethene	9.14	95	283272	9.38	ug/Kg	98
39) 1,2-dichloropropane	9.61	63	291923	9.60	ug/Kg	98
40) dibromomethane	9.82	93	182383	9.69	ug/Kg	98
41) bromodichloromethane	10.12	83	364826	10.06	ug/Kg	97
42) 2-Chloroethyl vinyl ether	11.38	63	93220m	185.21	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.21	43	319998	9.28	ug/Kg	97
44) cis-1,3-dichloropropene	10.91	75	387891	9.50	ug/Kg	100
46) toluene	11.38	92	631032	9.34	ug/Kg	96
47) trans-1,3-dichloropropene	11.97	75	327262	12.15	ug/Kg	99
48) 1,1,2-trichloroethane	12.29	83	217548	9.79	ug/Kg	97
50) 2-Hexanone	12.73	43	208683m	10.30	ug/Kg	95
51) tetrachloroethene	12.31	166	257117	9.30	ug/Kg	97
52) 1,3-dichloropropane	12.58	76	420603	9.14	ug/Kg	99
53) dibromochloromethane	12.93	129	258180	9.66	ug/Kg	98
54) 1,2-dibromoethane	13.11	107	248051	9.24	ug/Kg	96
55) chlorobenzene	13.99	112	702181	9.16	ug/Kg	95
56) 1,1,1,2-tetrachloroethane	14.18	131	229815	9.72	ug/Kg	97
57) ethylbenzene	14.14	91	1199077	9.19	ug/Kg	99
58) m,p-xylene	14.38	106	878908	18.40	ug/Kg	99
59) o-xylene	15.13	106	412816	8.86	ug/Kg	96
60) styrene	15.19	104	710261	8.99	ug/Kg	97
61) bromoform	15.57	173	161346	9.91	ug/Kg	94
64) isopropylbenzene	15.81	105	1138021	8.85	ug/Kg	99
65) bromobenzene	16.44	156	277810	9.10	ug/Kg	98
66) 1,1,2,2-tetrachloroethane	16.58	83	352538	9.62	ug/Kg	100
67) 1,2,3-trichloropropane	16.65	110	85634m	9.55	ug/Kg	94
68) n-propylbenzene	16.60	91	1388679	9.05	ug/Kg	98
69) 2-chlorotoluene	16.80	91	799219	8.54	ug/Kg	99
70) 4-chlorotoluene	17.03	91	934350	9.22	ug/Kg	96
71) 1,3,5-trimethylbenzene	16.97	105	914532	9.00	ug/Kg	100
72) tert-butylbenzene	17.55	91	561746	9.07	ug/Kg	96
73) 1,2,4-trimethylbenzene	17.69	105	906638	9.05	ug/Kg	98
74) sec-butylbenzene	17.99	105	1174527	8.90	ug/Kg	98
75) 1,3-dichlorobenzene	18.27	146	492273	9.02	ug/Kg	98
76) 4-isopropyltoluene	18.29	119	896971	8.98	ug/Kg	99
77) 1,4-dichlorobenzene	18.47	146	499896	9.12	ug/Kg	99

(#) = qualifier out of range (m) = manual integration

E2604.D 8260ES6.M Fri Apr 01 19:52:02 2005

Page 2

000104

Data File : C:\HPCHEM\1\DATA\040105\E2604.D

Vial: 3

Acq On : 1 Apr 05 9:32 am

Operator: xl

Sample : 10ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:27 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
78) 1,2-dichlorobenzene	19.24	146	467868	8.85 ug/Kg	98
79) n-butylbenzene	19.13	91	828004	8.74 ug/Kg	98
80) 1,2-dibromo-3-chloropropan	21.17	75	47912	12.24 ug/Kg	88
81) 1,2,4-trichlorobenzene	23.03	180	241022	8.68 ug/Kg	99
82) hexachlorobutadiene	23.31	225	126748	9.14 ug/Kg	98
83) naphthalene	23.56	128	624866	8.89 ug/Kg	100
84) 1,2,3-trichlorobenzene	24.11	180	252338	9.20 ug/Kg	99


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2604.D
Acq On : 1 Apr 05 9:32 am
Sample : 10ppb 8260s std
Misc : samp 8260_s
MS Integration Params: rteint.p
Quant Time: Apr 1 19:27 19105

Vial: 3
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

```
Method       : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
Title        : SW-846 Method 8260B
Last Update   : Fri Apr 01 19:18:41 2005
Response via  : Initial Calibration
```

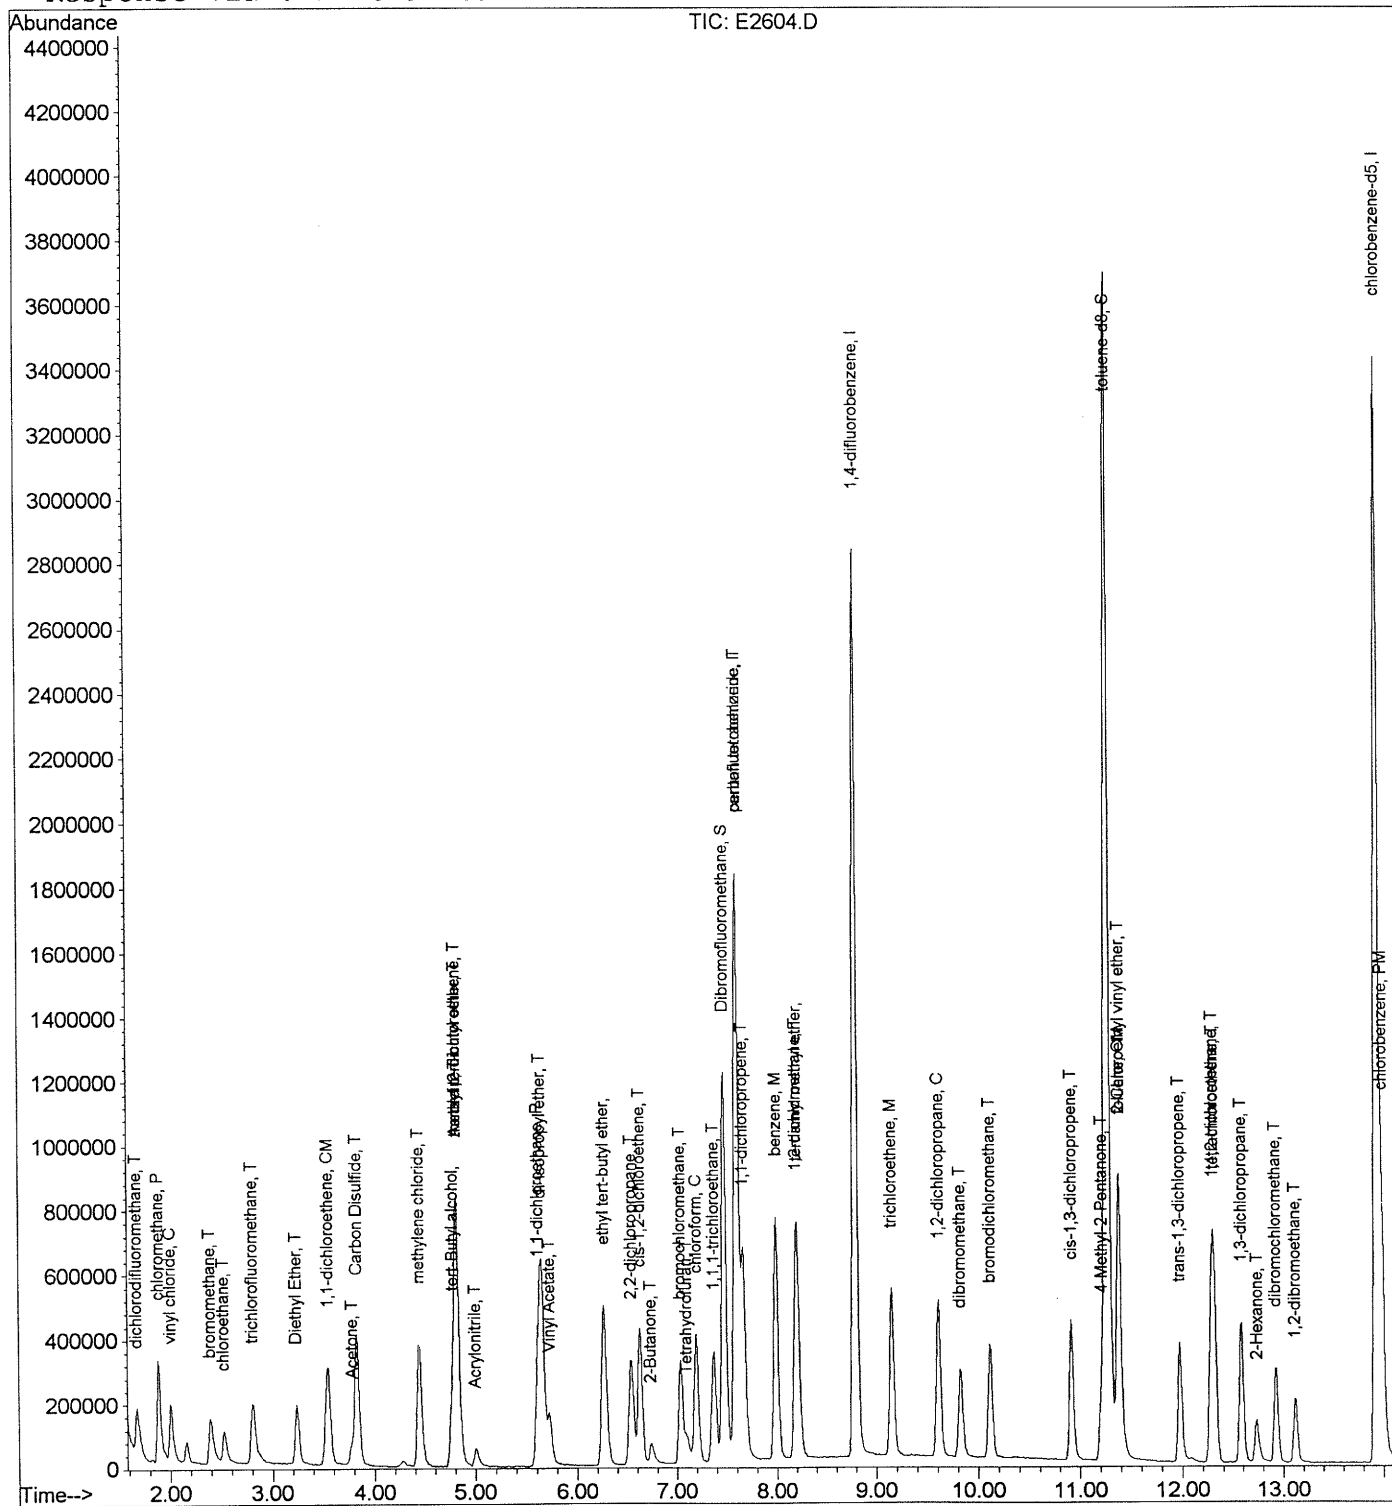


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2604.D
 Acq On : 1 Apr 05 9:32 am
 Sample : 10ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 19:27 19105

Vial: 3
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

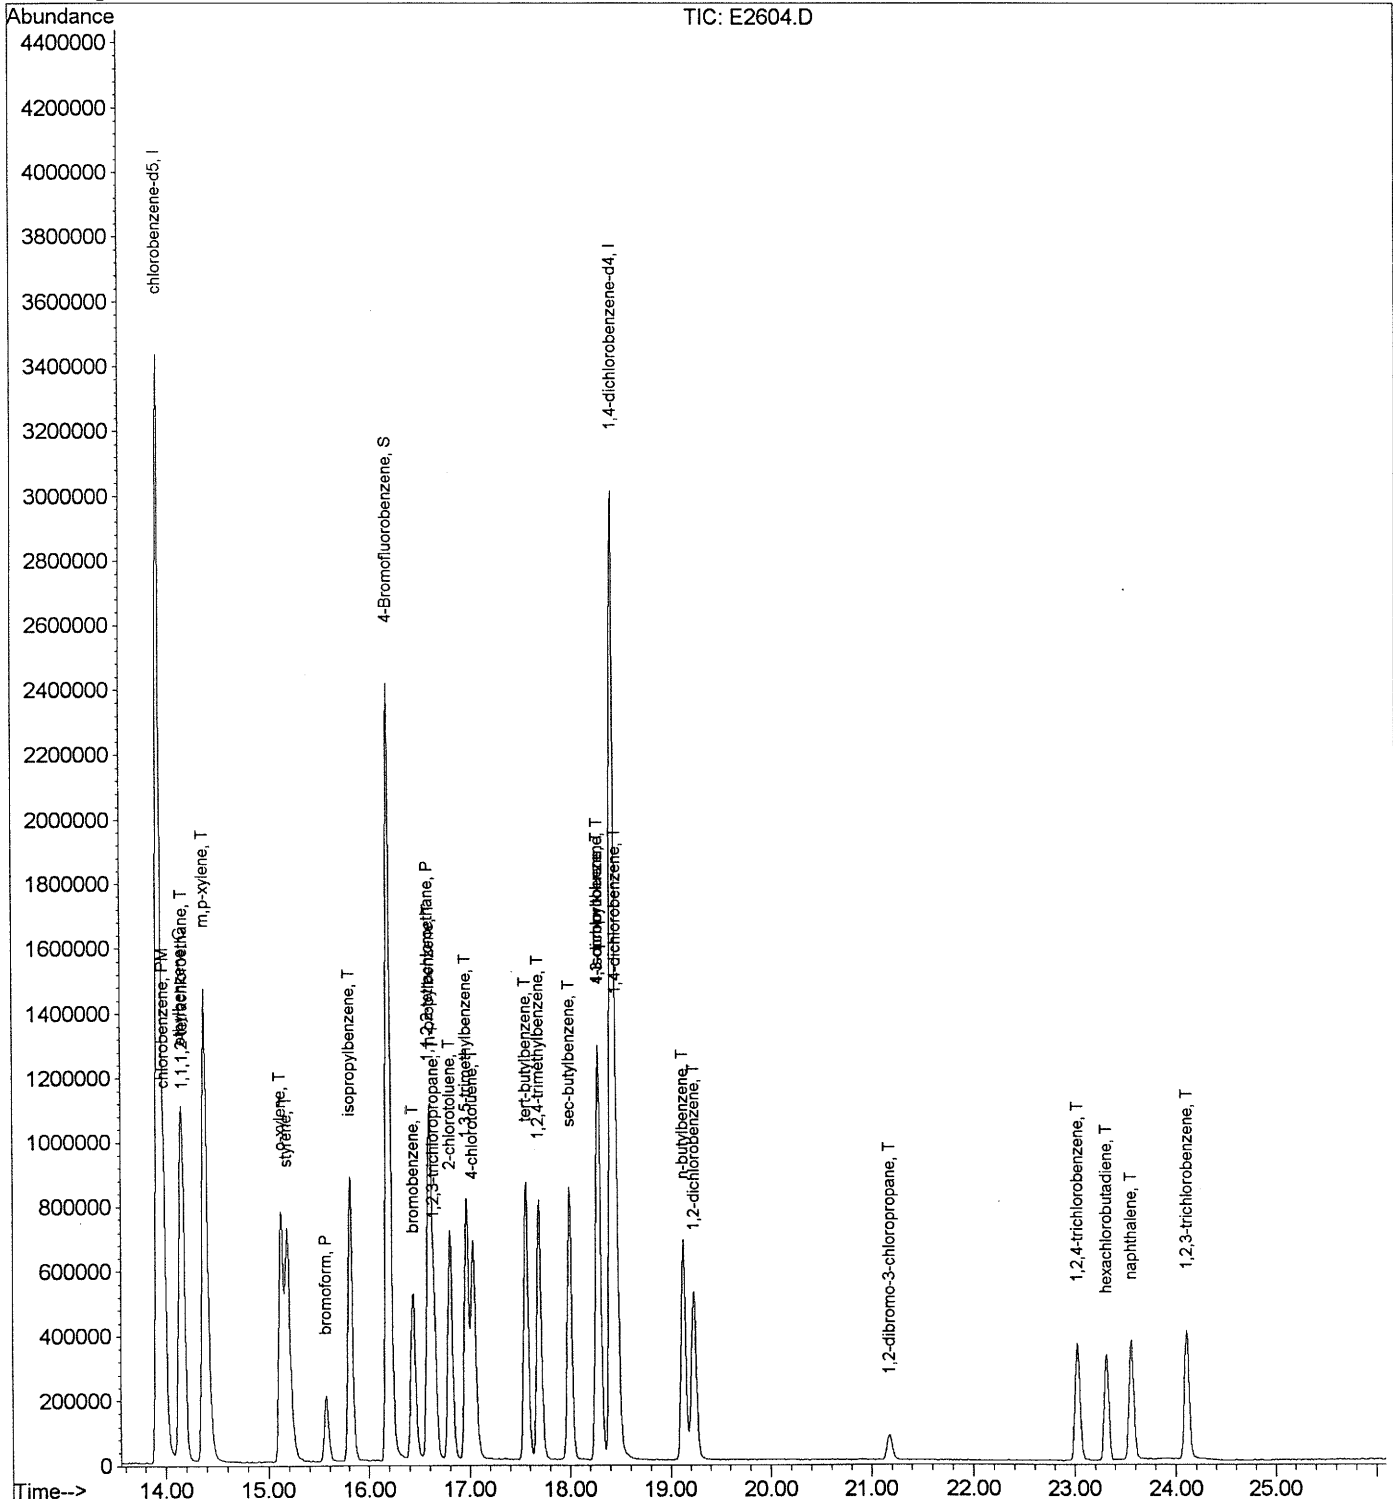

Data File : C:\HPCHEM\1\DATA\040105\E2605.D

Vial: 4

Acq On : 1 Apr 05 10:06 am

Operator: xl

Sample : 20ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:40 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.60	168	1866328	50.00	ug/Kg	-0.03
32) 1,4-difluorobenzene	8.79	114	3429808	50.00	ug/Kg	-0.03
49) chlorobenzene-d5	13.94	117	3242989	50.00	ug/Kg	-0.03
63) 1,4-dichlorobenzene-d4	18.42	152	1476397	50.00	ug/Kg	-0.03

System Monitoring Compounds

29) Dibromofluoromethane	7.47	113	1132692	47.11	ug/Kg	-0.03
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.22%		
45) toluene-d8	11.26	98	3997295	50.60	ug/Kg	-0.03
Spiked Amount 50.000	Range 81 - 120		Recovery =	101.20%		
62) 4-Bromofluorobenzene	16.20	95	1540447	50.29	ug/Kg	-0.03
Spiked Amount 50.000	Range 74 - 121		Recovery =	100.58%		

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.68	85	502275	26.61	ug/Kg	96
3) chloromethane	1.89	50	950906	21.16	ug/Kg	99
4) vinyl chloride	2.01	62	564475	20.39	ug/Kg	99
5) bromomethane	2.39	96	274597	31.82	ug/Kg	99
6) chloroethane	2.53	64	300095	19.19	ug/Kg	94
7) trichlorofluoromethane	2.81	101	557983	20.81	ug/Kg	99
8) Diethyl Ether	3.24	45	255832	17.33	ug/Kg	97
9) Acrolein	4.80	56	152277	87.40	ug/Kg	90
10) Acetone	3.77	43	192464m	16.92	ug/Kg	100
12) 1,1-dichloroethene	3.55	96	306354	17.68	ug/Kg	97
13) Iodomethane	3.79	142	90200m	15.73	ug/Kg	93
14) methylene chloride	4.45	84	555505	18.09	ug/Kg	98
15) Carbon Disulfide	3.83	76	1783354	17.78	ug/Kg	99
16) Acrylonitrile	4.99	53	162404	18.21	ug/Kg	95
17) tert-Butyl alcohol	4.77	59	608363	208.56	ug/Kg	100
18) methyl tert-butyl ether	4.82	73	1249772	18.93	ug/Kg	100
19) trans-1,2-dichloroethene	4.82	96	503369	18.46	ug/Kg	99
20) 1,1-dichloroethane	5.61	63	952682	18.00	ug/Kg	97
21) di-isopropyl ether	5.64	45	1861121	17.97	ug/Kg	99
22) Vinyl Acetate	5.72	43	831444	19.23	ug/Kg	98
23) ethyl tert-butyl ether	6.26	59	1449817	18.48	ug/Kg	99
24) 2-Butanone	6.73	43	299267	18.48	ug/Kg	98
25) 2,2-dichloropropane	6.54	77	592528	18.92	ug/Kg	98
26) cis-1,2-dichloroethene	6.63	96	558174	17.84	ug/Kg	95
27) bromochloromethane	7.04	128	264320	17.84	ug/Kg	97
28) chloroform	7.19	83	952236	18.30	ug/Kg	98
30) Tetrahydrofuran	7.08	42	174503	19.83	ug/Kg	99

(#) = qualifier out of range (m) = manual integration

E2605.D 8260ES6.M

Fri Apr 01 19:52:18 2005

4/1/05
xl

000108

Data File : C:\HPCHEM\1\DATA\040105\E2605.D

Vial: 4

Acq On : 1 Apr 05 10:06 am

Operator: xl

Sample : 20ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:40 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) 1,1,1-trichloroethane	7.37	97	669810	18.46	ug/Kg	99
33) carbon tetrachloride	7.59	117	675161	18.10	ug/Kg	99
34) 1,1-dichloropropene	7.66	75	932869	21.23	ug/Kg	100
35) benzene	7.99	78	2008315	18.29	ug/Kg	100
36) 1,2-dichloroethane	8.19	62	718825	19.53	ug/Kg	100
37) tert amyl methyl ether	8.20	73	1194621	20.18	ug/Kg	99
38) trichloroethene	9.15	95	560697	19.12	ug/Kg	97
39) 1,2-dichloropropane	9.60	63	565283	19.16	ug/Kg	99
40) dibromomethane	9.82	93	357999	19.60	ug/Kg	97
41) bromodichloromethane	10.12	83	707492	20.09	ug/Kg	98
42) 2-Chloroethyl vinyl ether	11.38	63	181232m	253.42	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.20	43	646732	19.32	ug/Kg	98
44) cis-1,3-dichloropropene	10.91	75	764857	19.29	ug/Kg	99
46) toluene	11.38	92	1250690	19.08	ug/Kg	99
47) trans-1,3-dichloropropene	11.97	75	667445	20.51	ug/Kg	99
48) 1,1,2-trichloroethane	12.28	83	430233	19.94	ug/Kg	98
50) 2-Hexanone	12.73	43	423898	18.48	ug/Kg	99
51) tetrachloroethene	12.32	166	507472	18.96	ug/Kg	97
52) 1,3-dichloropropane	12.58	76	830037	18.64	ug/Kg	95
53) dibromochloromethane	12.92	129	507553	19.62	ug/Kg	98
54) 1,2-dibromoethane	13.12	107	499591	19.24	ug/Kg	97
55) chlorobenzene	13.99	112	1364433	18.40	ug/Kg	98
56) 1,1,1,2-tetrachloroethane	14.17	131	447910	19.57	ug/Kg	99
57) ethylbenzene	14.15	91	2401822	19.03	ug/Kg	99
58) m,p-xylene	14.38	106	1746266	37.78	ug/Kg	99
59) o-xylene	15.13	106	842785	18.69	ug/Kg	99
60) styrene	15.19	104	1426162	18.66	ug/Kg	99
61) bromoform	15.57	173	315047	20.01	ug/Kg	96
64) isopropylbenzene	15.81	105	2310591	18.56	ug/Kg	99
65) bromobenzene	16.44	156	542486	18.35	ug/Kg	94
66) 1,1,2,2-tetrachloroethane	16.58	83	703922	19.84	ug/Kg	100
67) 1,2,3-trichloropropane	16.65	110	169770	19.54	ug/Kg	97
68) n-propylbenzene	16.60	91	2798246	18.82	ug/Kg	99
69) 2-chlorotoluene	16.81	91	1603849	17.70	ug/Kg	100
70) 4-chlorotoluene	17.04	91	1840972	18.77	ug/Kg	98
71) 1,3,5-trimethylbenzene	16.97	105	1847633	18.78	ug/Kg	97
72) tert-butylbenzene	17.56	91	1121243	18.69	ug/Kg	94
73) 1,2,4-trimethylbenzene	17.69	105	1804554	18.59	ug/Kg	98
74) sec-butylbenzene	18.00	105	2380074	18.63	ug/Kg	99
75) 1,3-dichlorobenzene	18.28	146	973441	18.43	ug/Kg	99
76) 4-isopropyltoluene	18.29	119	1808297	18.69	ug/Kg	99

(#)=qualifier out of range (m)=manual integration

E2605.D 8260ES6.M

Fri Apr 01 19:52:21 2005

Page 2

000109

Data File : C:\HPCHEM\1\DATA\040105\E2605.D

Vial: 4

Acq On : 1 Apr 05 10:06 am

Operator: xl

Sample : 20ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:40 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) 1,4-dichlorobenzene	18.47	146	990376	18.65	ug/Kg	97
78) 1,2-dichlorobenzene	19.24	146	952870	18.61	ug/Kg	98
79) n-butylbenzene	19.13	91	1673391	18.24	ug/Kg	98
80) 1,2-dibromo-3-chloropropan	21.18	75	96940	21.31	ug/Kg	95
81) 1,2,4-trichlorobenzene	23.03	180	523362	19.46	ug/Kg	98
82) hexachlorobutadiene	23.32	225	271488	20.21	ug/Kg	99
83) naphthalene	23.55	128	1403649	20.62	ug/Kg	100
84) 1,2,3-trichlorobenzene	24.11	180	536123	20.19	ug/Kg	99


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2605.D
Acq On : 1 Apr 05 10:06 am
Sample : 20ppb 8260s std
Misc : samp 8260_s
MS Integration Params: rteint.p
Quant Time: Apr 1 19:40 19105

Vial: 4
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Fri Apr 01 19:18:41 2005
Response via : Initial Calibration

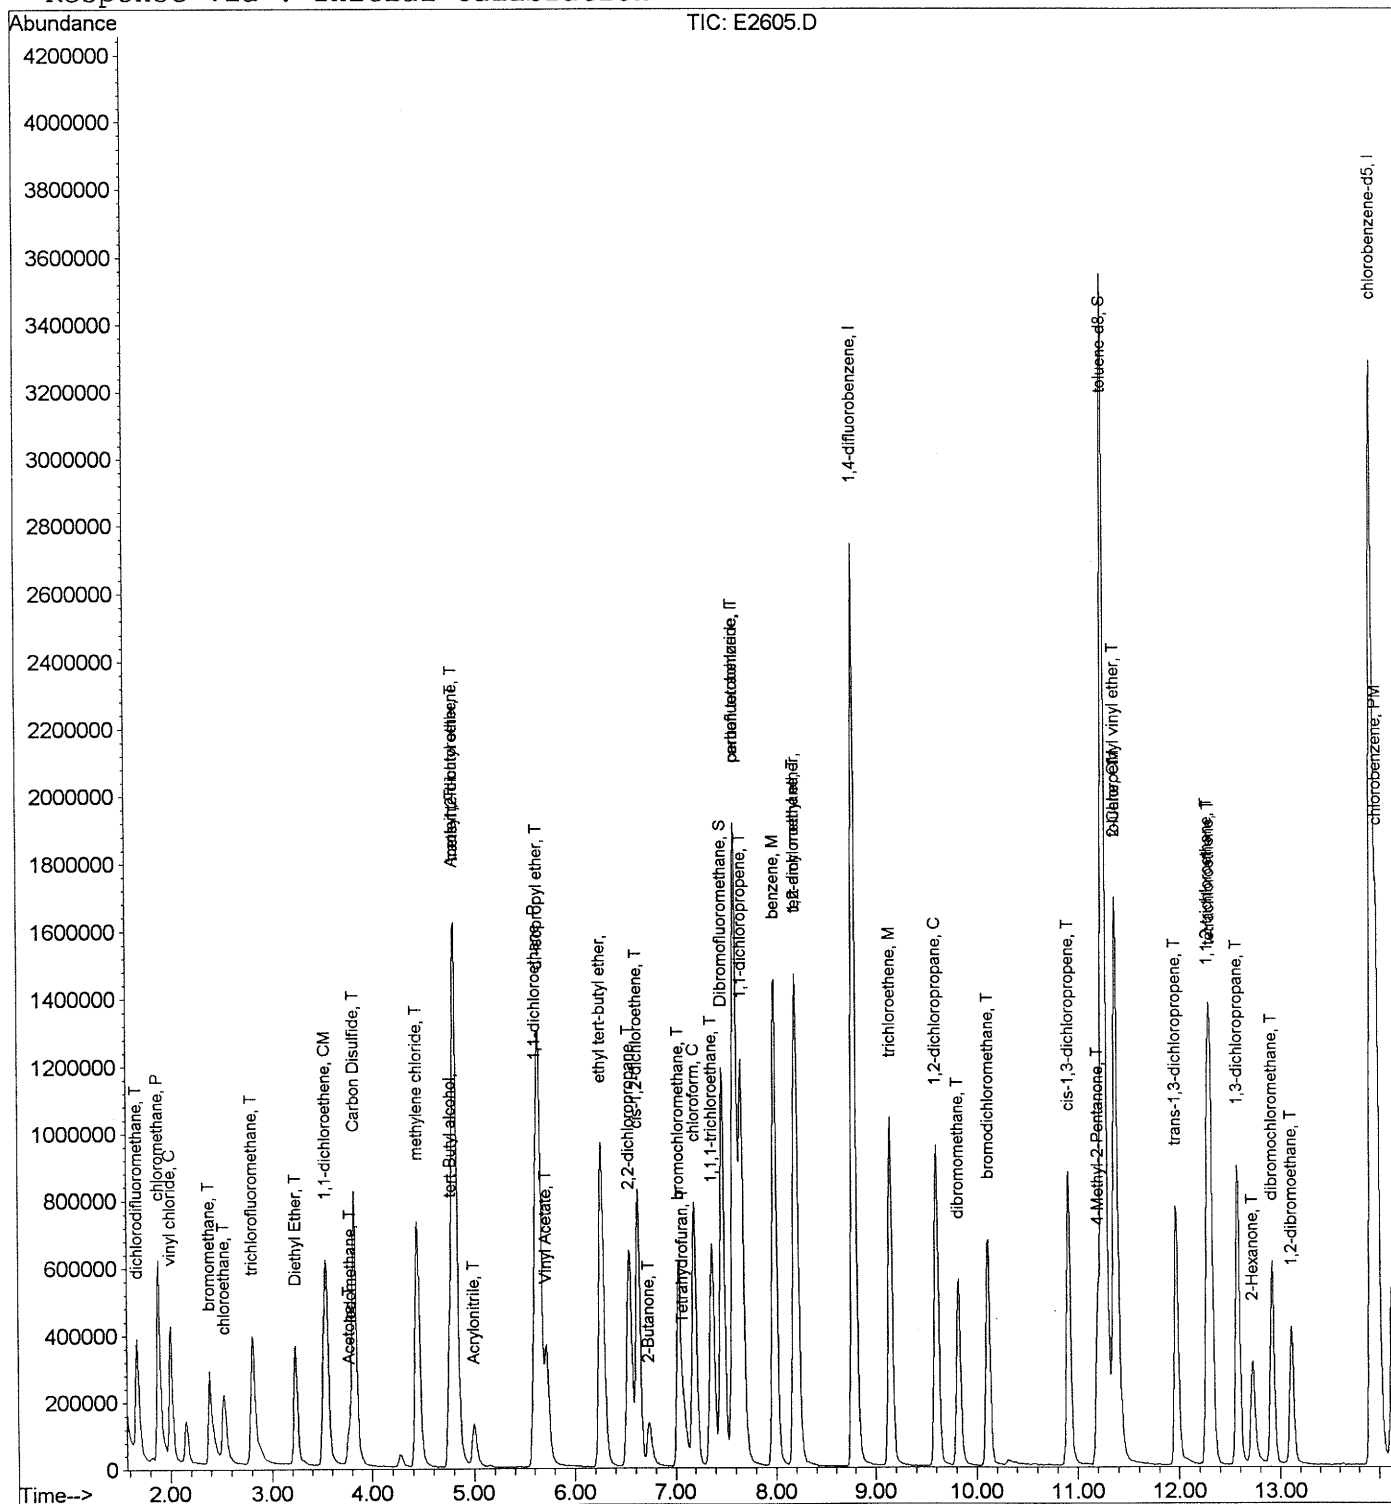

Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2605.D

Acq On : 1 Apr 05 10:06 am

Sample : 20ppb 8260s std

Misc : samp 8260_s

MS Integration Params: rteint.p

Quant Time: Apr 1 19:40 19105

Vial: 4

Operator: xl

Inst : inst e

Multiplr: 1.00


Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Fri Apr 01 19:18:41 2005

Response via : Initial Calibration

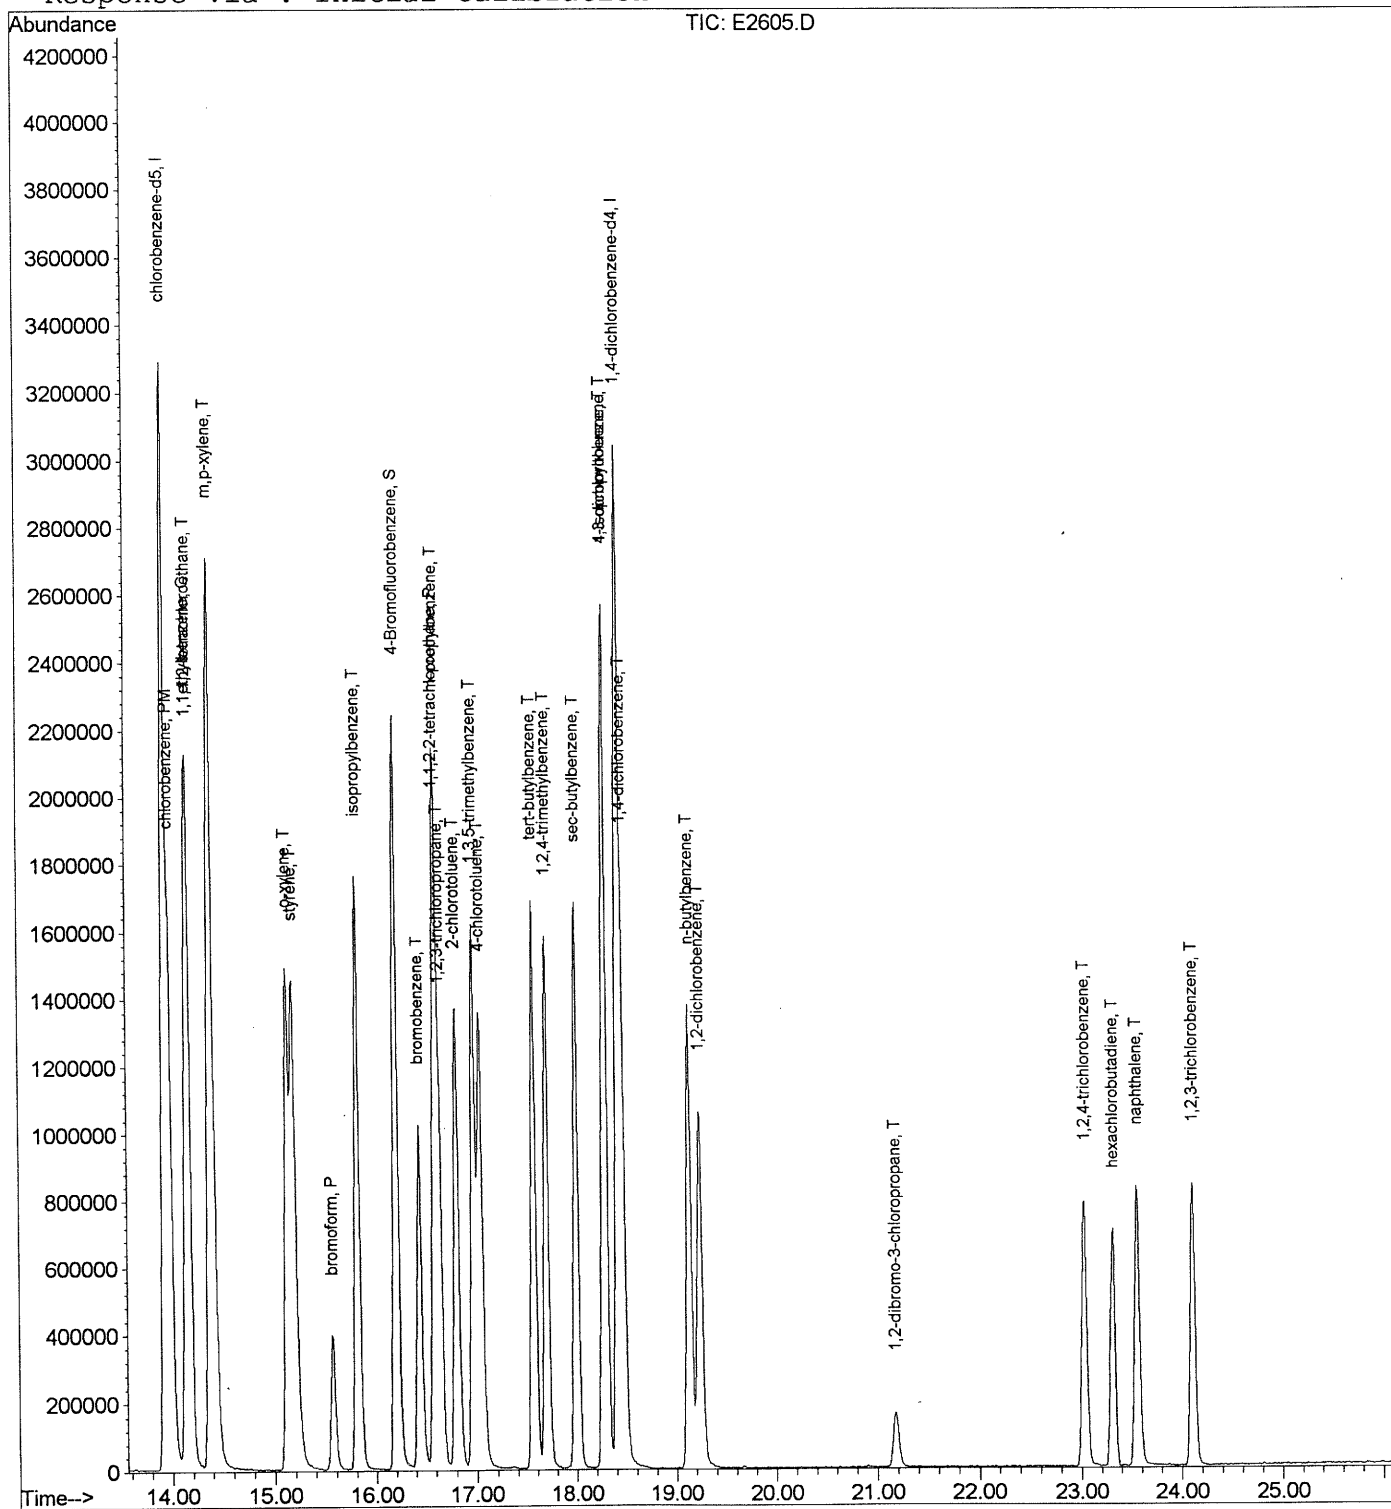

Data File : C:\HPCHEM\1\DATA\040105\E2606.D

Vial: 5

Acq On : 1 Apr 05 10:40 am

Operator: xl

Sample : 50ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 11:40 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.61	168	1918584	50.00	ug/Kg	-0.02
32) 1,4-difluorobenzene	8.79	114	3610022	50.00	ug/Kg	-0.03
49) chlorobenzene-d5	13.93	117	3474140	50.00	ug/Kg	-0.03
63) 1,4-dichlorobenzene-d4	18.42	152	1595312	50.00	ug/Kg	-0.03

System Monitoring Compounds

29) Dibromofluoromethane	7.47	113	1213878	49.11	ug/Kg	-0.03
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.22%		
45) toluene-d8	11.26	98	4253406	51.15	ug/Kg	-0.03
Spiked Amount 50.000	Range 81 - 120		Recovery =	102.30%		
62) 4-Bromofluorobenzene	16.19	95	1663996	50.71	ug/Kg	-0.03
Spiked Amount 50.000	Range 74 - 121		Recovery =	101.42%		

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.68	85	1270937	65.50	ug/Kg	98
3) chloromethane	1.89	50	2417336	52.32	ug/Kg	98
4) vinyl chloride	2.01	62	1455833	51.16	ug/Kg	98
5) bromomethane	2.38	96	239996	23.25	ug/Kg	99
6) chloroethane	2.51	64	762259	47.43	ug/Kg	97
7) trichlorofluoromethane	2.81	101	1418899	51.48	ug/Kg	99
8) Diethyl Ether	3.23	45	680398	44.82	ug/Kg	96
10) Acetone	3.77	43	508589	43.50	ug/Kg	99
12) 1,1-dichloroethene	3.55	96	804747	45.19	ug/Kg	95
13) Iodomethane	3.80	142	264178	53.48	ug/Kg	95
14) methylene chloride	4.45	84	1444211	45.75	ug/Kg	100
15) Carbon Disulfide	3.83	76	4735934	45.94	ug/Kg	99
16) Acrylonitrile	5.00	53	437723	47.74	ug/Kg	98
17) tert-Butyl alcohol	4.76	59	1661984	540.41	ug/Kg	100
18) methyl tert-butyl ether	4.81	73	3382498	49.84	ug/Kg	100
19) trans-1,2-dichloroethene	4.82	96	1308933	46.69	ug/Kg	99
20) 1,1-dichloroethane	5.61	63	2502340	46.00	ug/Kg	99
21) di-isopropyl ether	5.65	45	5006263	47.02	ug/Kg	100
22) Vinyl Acetate	5.72	43	2251187	50.64	ug/Kg	100
23) ethyl tert-butyl ether	6.26	59	3976372	49.31	ug/Kg	100
24) 2-Butanone	6.73	43	835910	50.21	ug/Kg	99
25) 2,2-dichloropropane	6.54	77	1571853	48.82	ug/Kg	97
26) cis-1,2-dichloroethene	6.63	96	1492847	46.41	ug/Kg	97
27) bromochloromethane	7.04	128	709239	46.58	ug/Kg	97
28) chloroform	7.19	83	2488387	46.51	ug/Kg	98
30) Tetrahydrofuran	7.07	42	458212	50.65	ug/Kg	95
31) 1,1,1-trichloroethane	7.37	97	1789908	47.99	ug/Kg	99

(#) = qualifier out of range (m) = manual integration

E2606.D 8260ES6.M

Fri Apr 01 19:52:43 2005

Page 1

000113

Data File : C:\HPCHEM\1\DATA\040105\E2606.D

Vial: 5

Acq On : 1 Apr 05 10:40 am

Operator: xl

Sample : 50ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 11:40 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) carbon tetrachloride	7.59	117	1541784	46.86	ug/Kg	90
34) 1,1-dichloropropene	7.66	75	2160419	46.72	ug/Kg	99
35) benzene	7.99	78	5380933	46.55	ug/Kg	99
36) 1,2-dichloroethane	8.19	62	1919021	49.53	ug/Kg	99
37) tert amyl methyl ether	8.20	73	3298783	52.95	ug/Kg	99
38) trichloroethene	9.15	95	1506583	48.82	ug/Kg	98
39) 1,2-dichloropropane	9.61	63	1523972	49.07	ug/Kg	99
40) dibromomethane	9.82	93	978336	50.88	ug/Kg	100
41) bromodichloromethane	10.11	83	1923257	51.89	ug/Kg	98
42) 2-Chloroethyl vinyl ether	11.38	63	477675m	388.39	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.20	43	1790150	50.80	ug/Kg	97
44) cis-1,3-dichloropropene	10.91	75	2189961	52.48	ug/Kg	99
46) toluene	11.38	92	3308939	47.95	ug/Kg	95
47) trans-1,3-dichloropropene	11.97	75	1924700	48.25	ug/Kg	100
48) 1,1,2-trichloroethane	12.28	83	1175203	51.76	ug/Kg	99
50) 2-Hexanone	12.72	43	1279072	46.88	ug/Kg	97
51) tetrachloroethene	12.31	166	1326910	46.28	ug/Kg	96
52) 1,3-dichloropropane	12.58	76	2299757	48.21	ug/Kg	99
53) dibromochloromethane	12.92	129	1425951	51.45	ug/Kg	99
54) 1,2-dibromoethane	13.11	107	1387173	49.87	ug/Kg	100
55) chlorobenzene	13.99	112	3653523	45.99	ug/Kg	98
56) 1,1,1,2-tetrachloroethane	14.17	131	1207552	49.25	ug/Kg	98
57) ethylbenzene	14.14	91	6433734	47.58	ug/Kg	99
58) m,p-xylene	14.39	106	4643929	93.78	ug/Kg	98
59) o-xylene	15.13	106	2244664	46.48	ug/Kg	97
60) styrene	15.19	104	3926020	47.95	ug/Kg	99
61) bromoform	15.57	173	897577	53.21	ug/Kg	99
64) isopropylbenzene	15.81	105	6193344	46.04	ug/Kg	100
65) bromobenzene	16.44	156	1482208	46.41	ug/Kg	96
66) 1,1,2,2-tetrachloroethane	16.58	83	1901154	49.60	ug/Kg	99
67) 1,2,3-trichloropropane	16.65	110	464917	49.53	ug/Kg	93
68) n-propylbenzene	16.61	91	7496186	46.66	ug/Kg	99
69) 2-chlorotoluene	16.80	91	4295712	43.88	ug/Kg	99
70) 4-chlorotoluene	17.04	91	4857115	45.82	ug/Kg	98
71) 1,3,5-trimethylbenzene	16.97	105	4904363	46.14	ug/Kg	99
72) tert-butylbenzene	17.56	91	2975199	45.90	ug/Kg	92
73) 1,2,4-trimethylbenzene	17.69	105	4812089	45.88	ug/Kg	99
74) sec-butylbenzene	17.99	105	6427717	46.55	ug/Kg	98
75) 1,3-dichlorobenzene	18.27	146	2601977	45.59	ug/Kg	99
76) 4-isopropyltoluene	18.29	119	4886868	46.75	ug/Kg	98
77) 1,4-dichlorobenzene	18.46	146	2614083	45.56	ug/Kg	98

(#) = qualifier out of range (m) = manual integration

E2606.D 8260ES6.M

Fri Apr 01 19:52:46 2005

000114 Page 2

Data File : C:\HPCHEM\1\DATA\040105\E2606.D

Vial: 5

Acq On : 1 Apr 05 10:40 am

Operator: xl

Sample : 50ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 11:40 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
78) 1,2-dichlorobenzene	19.23	146	2563252	46.33	ug/Kg	98
79) n-butylbenzene	19.13	91	4611925	46.52	ug/Kg	100
80) 1,2-dibromo-3-chloropropan	21.17	75	280137	50.41	ug/Kg	96
81) 1,2,4-trichlorobenzene	23.02	180	1420801	48.90	ug/Kg	99
82) hexachlorobutadiene	23.31	225	693909	47.80	ug/Kg	99
83) naphthalene	23.56	128	4046700	55.02	ug/Kg	100
84) 1,2,3-trichlorobenzene	24.10	180	1424568	49.64	ug/Kg	98


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2606.D
 Acq On : 1 Apr 05 10:40 am
 Sample : 50ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 11:40 19105

Vial: 5
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

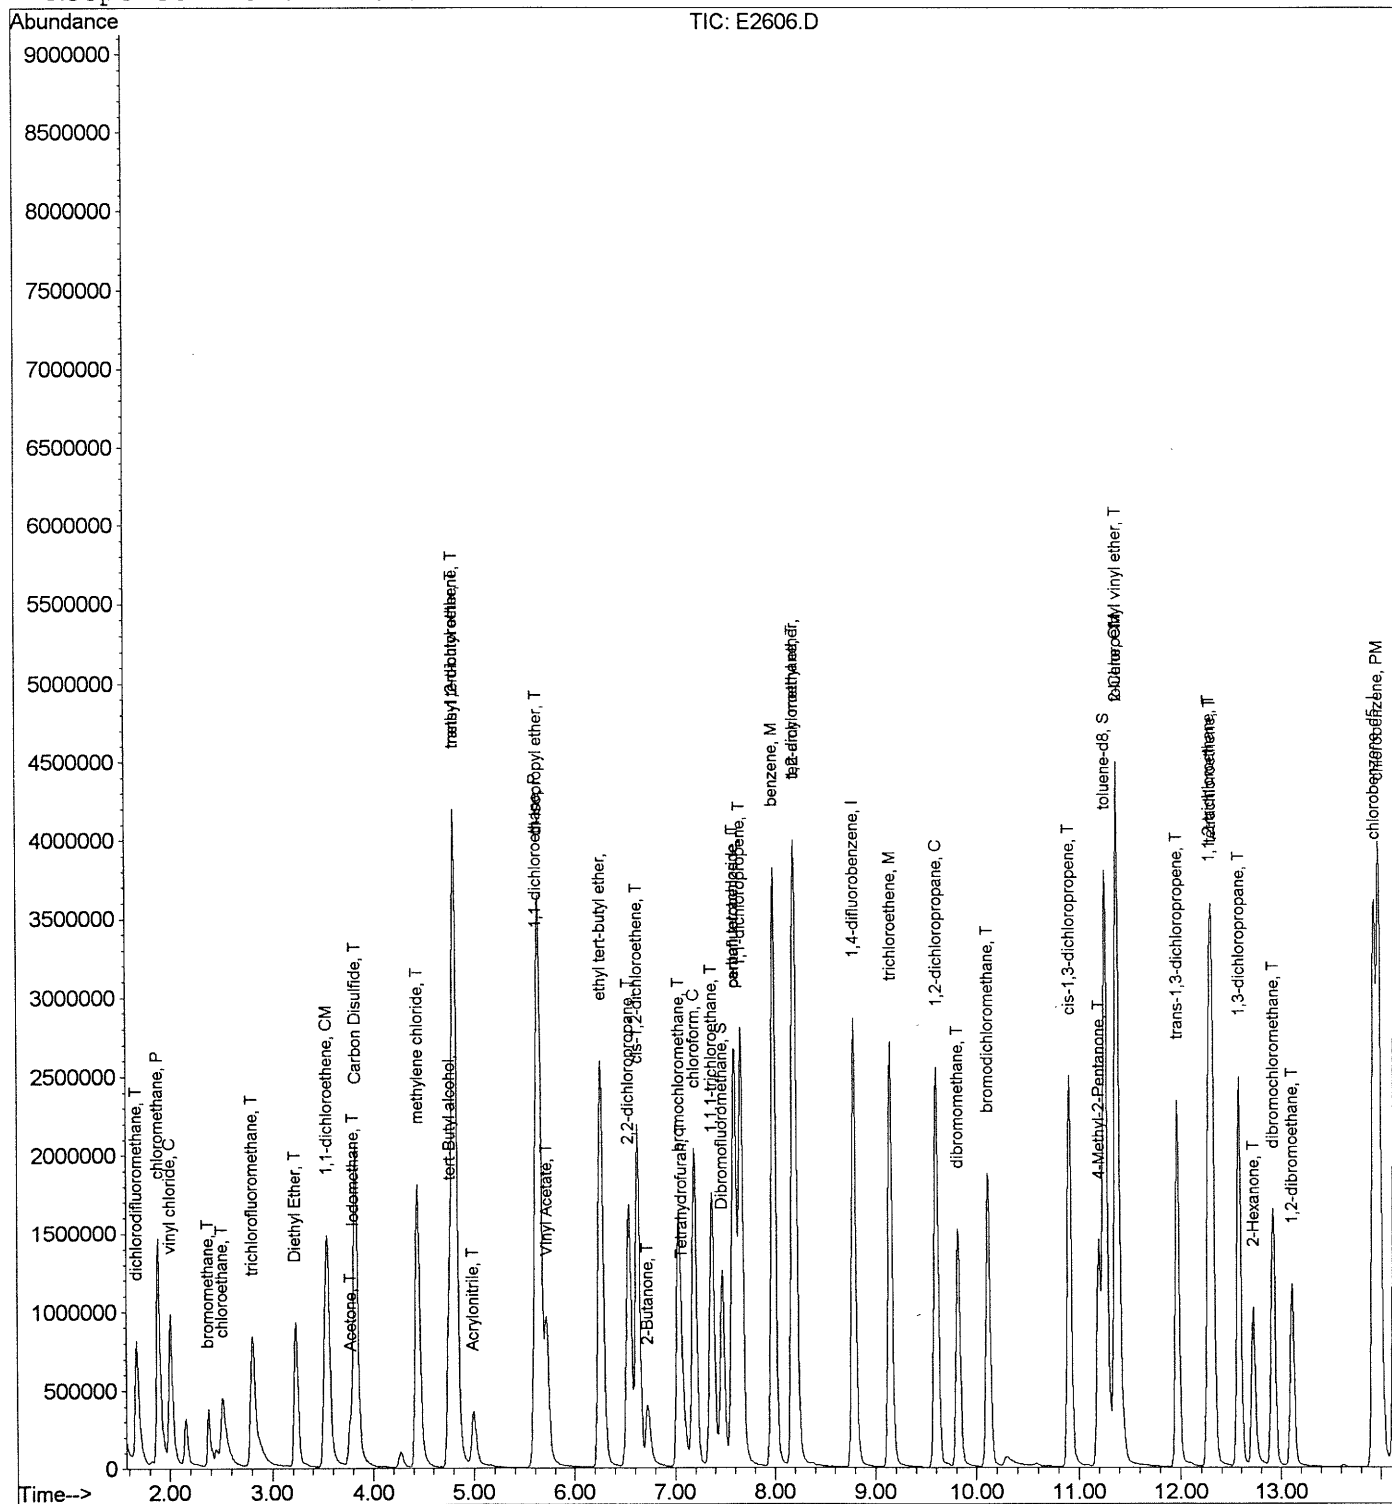


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2606.D
 Acq On : 1 Apr 05 10:40 am
 Sample : 50ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 11:40 19105

Vial: 5
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

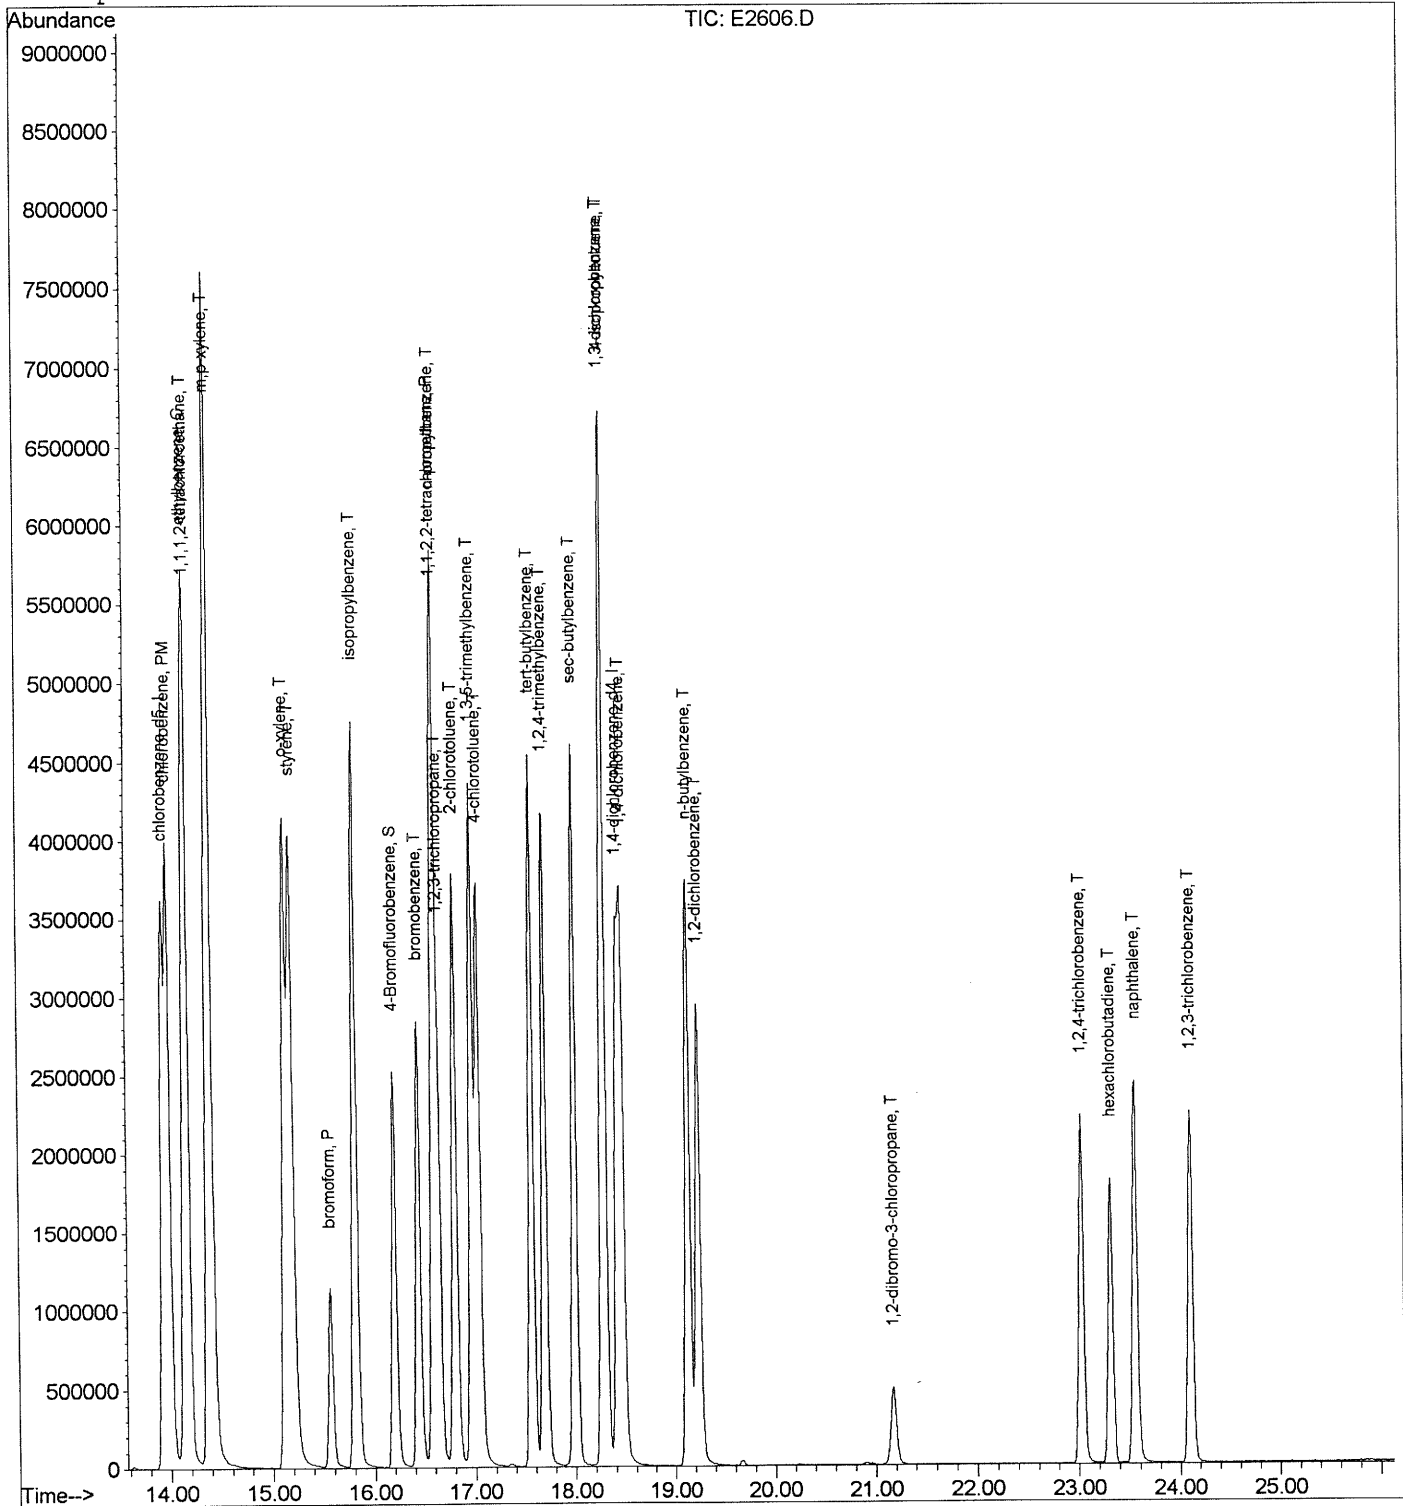

Data File : C:\HPCHEM\1\DATA\040105\E2607.D
 Acq On : 1 Apr 05 11:14 am
 Sample : 100ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 19:42 19105

Vial: 6
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Mar 14 14:14:50 2005
 Response via : Initial Calibration
 DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.60	168	1934377	50.00	ug/Kg	-0.03
32) 1,4-difluorobenzene	8.79	114	3683991	50.00	ug/Kg	-0.03
49) chlorobenzene-d5	13.94	117	3447529	50.00	ug/Kg	-0.02
63) 1,4-dichlorobenzene-d4	18.42	152	1637360	50.00	ug/Kg	-0.03

System Monitoring Compounds

29) Dibromofluoromethane	7.47	113	1222220	49.04	ug/Kg	-0.03
Spiked Amount 50.000	Range 80 - 120		Recovery	=	98.08%	
45) toluene-d8	11.26	98	4309185	50.78	ug/Kg	-0.03
Spiked Amount 50.000	Range 81 - 120		Recovery	=	101.56%	
62) 4-Bromofluorobenzene	16.19	95	1710578	52.53	ug/Kg	-0.03
Spiked Amount 50.000	Range 74 - 121		Recovery	=	105.06%	

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.67	85	2692751	137.64	ug/Kg	98
3) chloromethane	1.88	50	4953971	106.34	ug/Kg	97
4) vinyl chloride	2.01	62	3128899	109.06	ug/Kg	99
5) bromomethane	2.38	96	460443	71.53	ug/Kg	99
6) chloroethane	2.50	64	1270622	78.41	ug/Kg	98
7) trichlorofluoromethane	2.80	101	2976245	107.10	ug/Kg	99
8) Diethyl Ether	3.23	45	1383632	90.41	ug/Kg	99
10) Acetone	3.77	43	963730m	81.76	ug/Kg	100
12) 1,1-dichloroethene	3.54	96	1658447	92.36	ug/Kg	96
13) Iodomethane	3.79	142	571477m	96.09	ug/Kg	92
14) methylene chloride	4.45	84	3005391	94.43	ug/Kg	99
15) Carbon Disulfide	3.83	76	10104650	97.22	ug/Kg	98
16) Acrylonitrile	5.00	53	915562	99.05	ug/Kg	97
17) tert-Butyl alcohol	4.76	59	3250323	1040.41	ug/Kg	100
18) methyl tert-butyl ether	4.81	73	6971036	101.89	ug/Kg	100
19) trans-1,2-dichloroethene	4.82	96	2722506	96.32	ug/Kg	97
20) 1,1-dichloroethane	5.61	63	5231365	95.39	ug/Kg	98
21) di-isopropyl ether	5.65	45	10680276	99.49	ug/Kg	97
22) Vinyl Acetate	5.72	43	5003089	111.63	ug/Kg	99
23) ethyl tert-butyl ether	6.25	59	8495410	104.49	ug/Kg	100
24) 2-Butanone	6.72	43	1608218	95.81	ug/Kg	100
25) 2,2-dichloropropane	6.54	77	3371835	103.87	ug/Kg	98
26) cis-1,2-dichloroethene	6.63	96	3134394	96.65	ug/Kg	100
27) bromochloromethane	7.04	128	1475583	96.12	ug/Kg	99
28) chloroform	7.19	83	5286287	97.99	ug/Kg	99
30) Tetrahydrofuran	7.06	42	892494	97.86	ug/Kg	98
31) 1,1,1-trichloroethane	7.37	97	3762230	100.05	ug/Kg	98

(#) = qualifier out of range (m) = manual integration

Data File : C:\HPCHEM\1\DATA\040105\E2607.D

Vial: 6

Acq On : 1 Apr 05 11:14 am

Operator: xl

Sample : 100ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:42 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) carbon tetrachloride	7.58	117	3141197m	100.03	ug/Kg	80
34) 1,1-dichloropropene	7.66	75	4375646	92.72	ug/Kg	99
35) benzene	7.98	78	11481206	97.32	ug/Kg	98
36) 1,2-dichloroethane	8.18	62	3895067	98.51	ug/Kg	99
37) tert amyl methyl ether	8.20	73	7040158	110.74	ug/Kg	99
38) trichloroethene	9.15	95	3156193	100.21	ug/Kg	99
39) 1,2-dichloropropane	9.61	63	3273033	103.27	ug/Kg	100
40) dibromomethane	9.82	93	2039770	103.94	ug/Kg	98
41) bromodichloromethane	10.11	83	4114728	108.79	ug/Kg	99
42) 2-Chloroethyl vinyl ether	11.38	63	988828m	543.74	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.19	43	3632155	101.01	ug/Kg	97
44) cis-1,3-dichloropropene	10.91	75	4733494	111.15	ug/Kg	100
46) toluene	11.38	92	7051198	100.13	ug/Kg	96
47) trans-1,3-dichloropropene	11.97	75	4187964	97.72	ug/Kg	99
48) 1,1,2-trichloroethane	12.28	83	2440222	105.31	ug/Kg	97
50) 2-Hexanone	12.72	43	2659532	95.10	ug/Kg	98
51) tetrachloroethene	12.32	166	2752506	96.75	ug/Kg	96
52) 1,3-dichloropropane	12.58	76	4776978	100.91	ug/Kg	98
53) dibromochloromethane	12.92	129	3011411	109.50	ug/Kg	97
54) 1,2-dibromoethane	13.11	107	2910280	105.43	ug/Kg	97
55) chlorobenzene	13.99	112	7693820	97.60	ug/Kg	96
56) 1,1,1,2-tetrachloroethane	14.17	131	2525861	103.82	ug/Kg	98
57) ethylbenzene	14.15	91	13717992	102.24	ug/Kg	99
58) m,p-xylene	14.39	106	9584831	195.05	ug/Kg	96
59) o-xylene	15.13	106	4794156	100.03	ug/Kg	98
60) styrene	15.19	104	8426415	103.71	ug/Kg	96
61) bromoform	15.57	173	1915191	114.41	ug/Kg	96
64) isopropylbenzene	15.81	105	13405680	97.11	ug/Kg	98
65) bromobenzene	16.44	156	3143094	95.89	ug/Kg	96
66) 1,1,2,2-tetrachloroethane	16.58	83	3919198	99.62	ug/Kg	99
67) 1,2,3-trichloropropane	16.65	110	924845m	95.99	ug/Kg	90
68) n-propylbenzene	16.61	91	16390093	99.41	ug/Kg	97
69) 2-chlorotoluene	16.80	91	9221657	91.78	ug/Kg	99
70) 4-chlorotoluene	17.04	91	10413643	95.72	ug/Kg	98
71) 1,3,5-trimethylbenzene	16.97	105	10519505	96.43	ug/Kg	99
72) tert-butylbenzene	17.56	91	6332306	95.17	ug/Kg	96
73) 1,2,4-trimethylbenzene	17.70	105	10403359	96.65	ug/Kg	99
74) sec-butylbenzene	18.00	105	14039533	99.07	ug/Kg	97
75) 1,3-dichlorobenzene	18.27	146	5542017	94.61	ug/Kg	99
76) 4-isopropyltoluene	18.29	119	10556232	98.39	ug/Kg	97
77) 1,4-dichlorobenzene	18.46	146	5536607	94.02	ug/Kg	99

(#)=qualifier out of range (m)=manual integration

Data File : C:\HPCHEM\1\DATA\040105\E2607.D

Vial: 6

Acq On : 1 Apr 05 11:14 am

Operator: xl

Sample : 100ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:42 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Mar 14 14:14:50 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
78) 1,2-dichlorobenzene	19.23	146	5456214	96.10	ug/Kg	97
79) n-butylbenzene	19.13	91	10054450	98.81	ug/Kg	98
80) 1,2-dibromo-3-chloropropan	21.17	75	580495	97.79	ug/Kg	99
81) 1,2,4-trichlorobenzene	23.02	180	3049120	102.25	ug/Kg	97
82) hexachlorobutadiene	23.32	225	1489898	100.00	ug/Kg	99
83) naphthalene	23.56	128	8474295	112.26	ug/Kg	100
84) 1,2,3-trichlorobenzene	24.10	180	3072725	104.32	ug/Kg	99

XL 4/6/05


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2607.D
 Acq On : 1 Apr 05 11:14 am
 Sample : 100ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 19:42 19105

Vial: 6
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

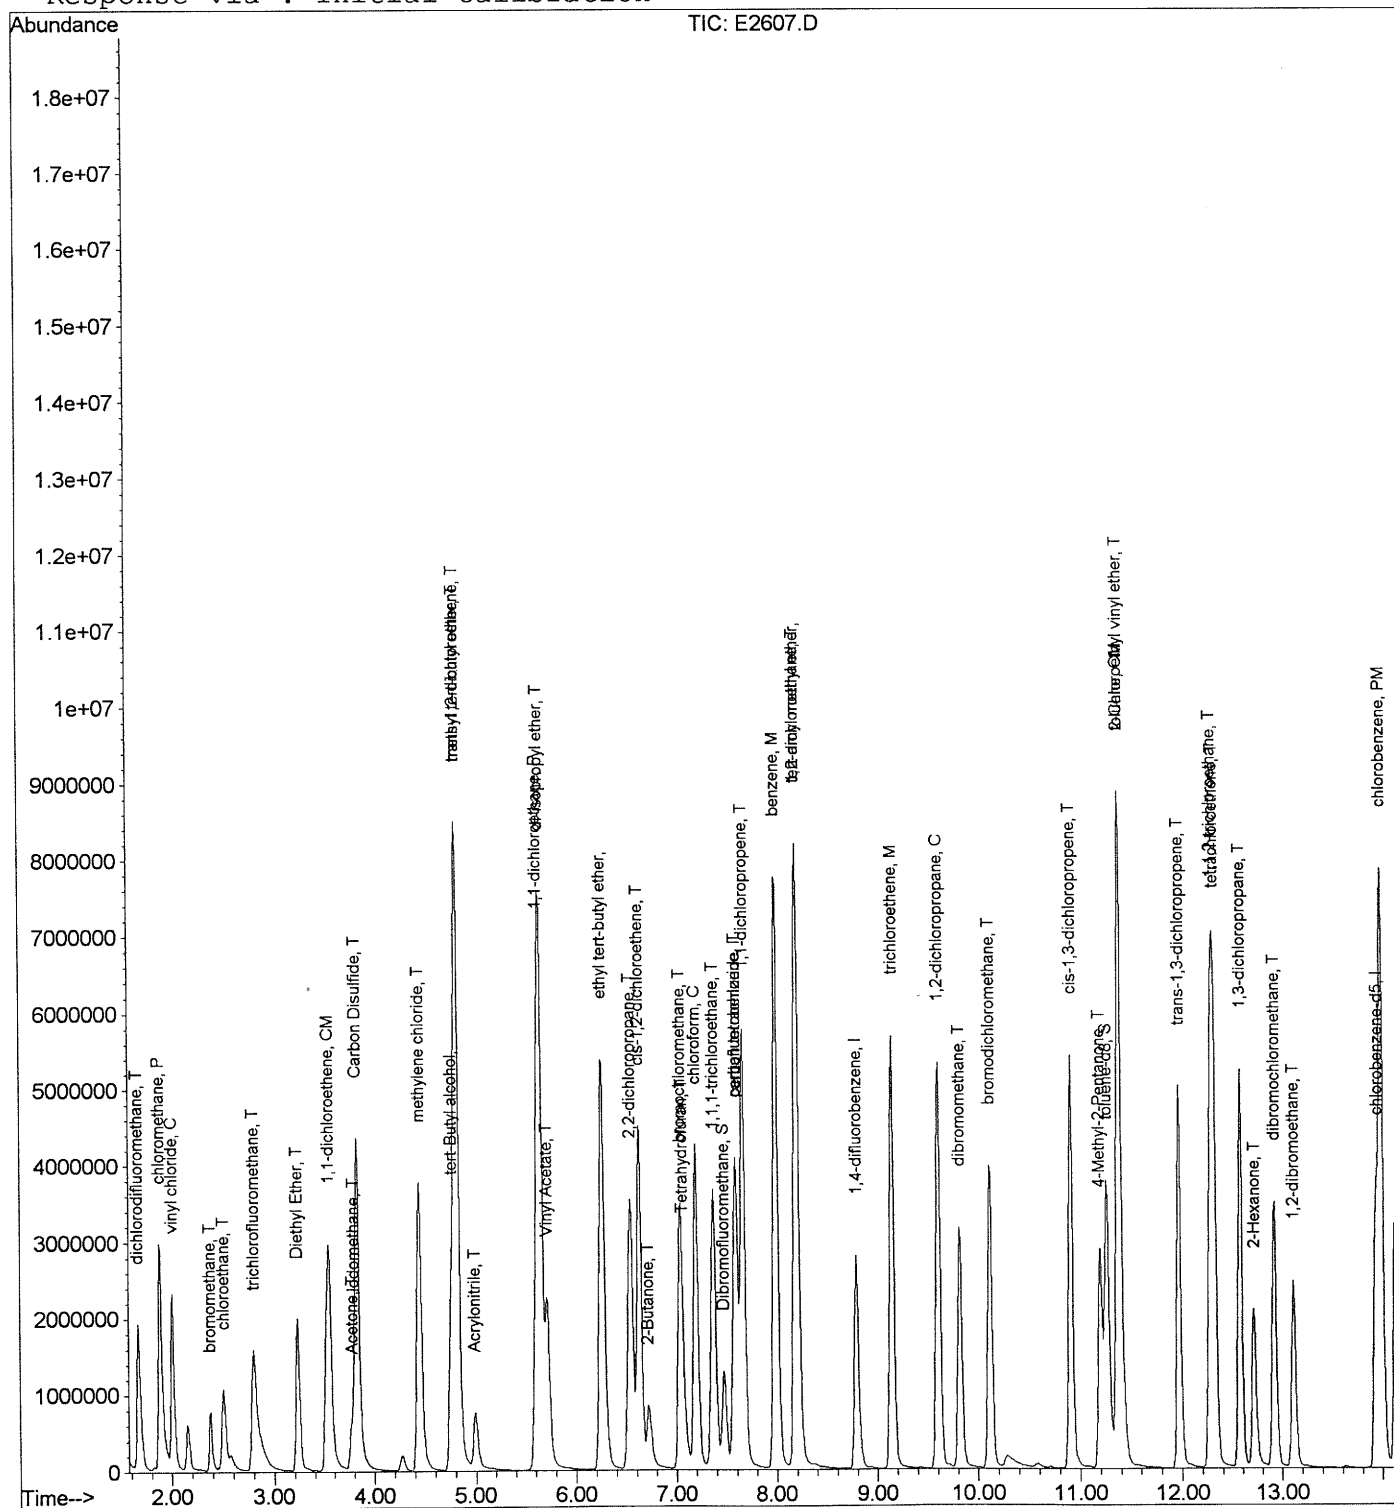

Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2607.D

Acq On : 1 Apr 05 11:14 am

Sample : 100ppb 8260s std

Misc : samp 8260_s

MS Integration Params: rteint.p

Quant Time: Apr 1 19:42 19105

Vial: 6

Operator: xl

Inst : inst e

Multiplr: 1.00


Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Fri Apr 01 19:18:41 2005

Response via : Initial Calibration

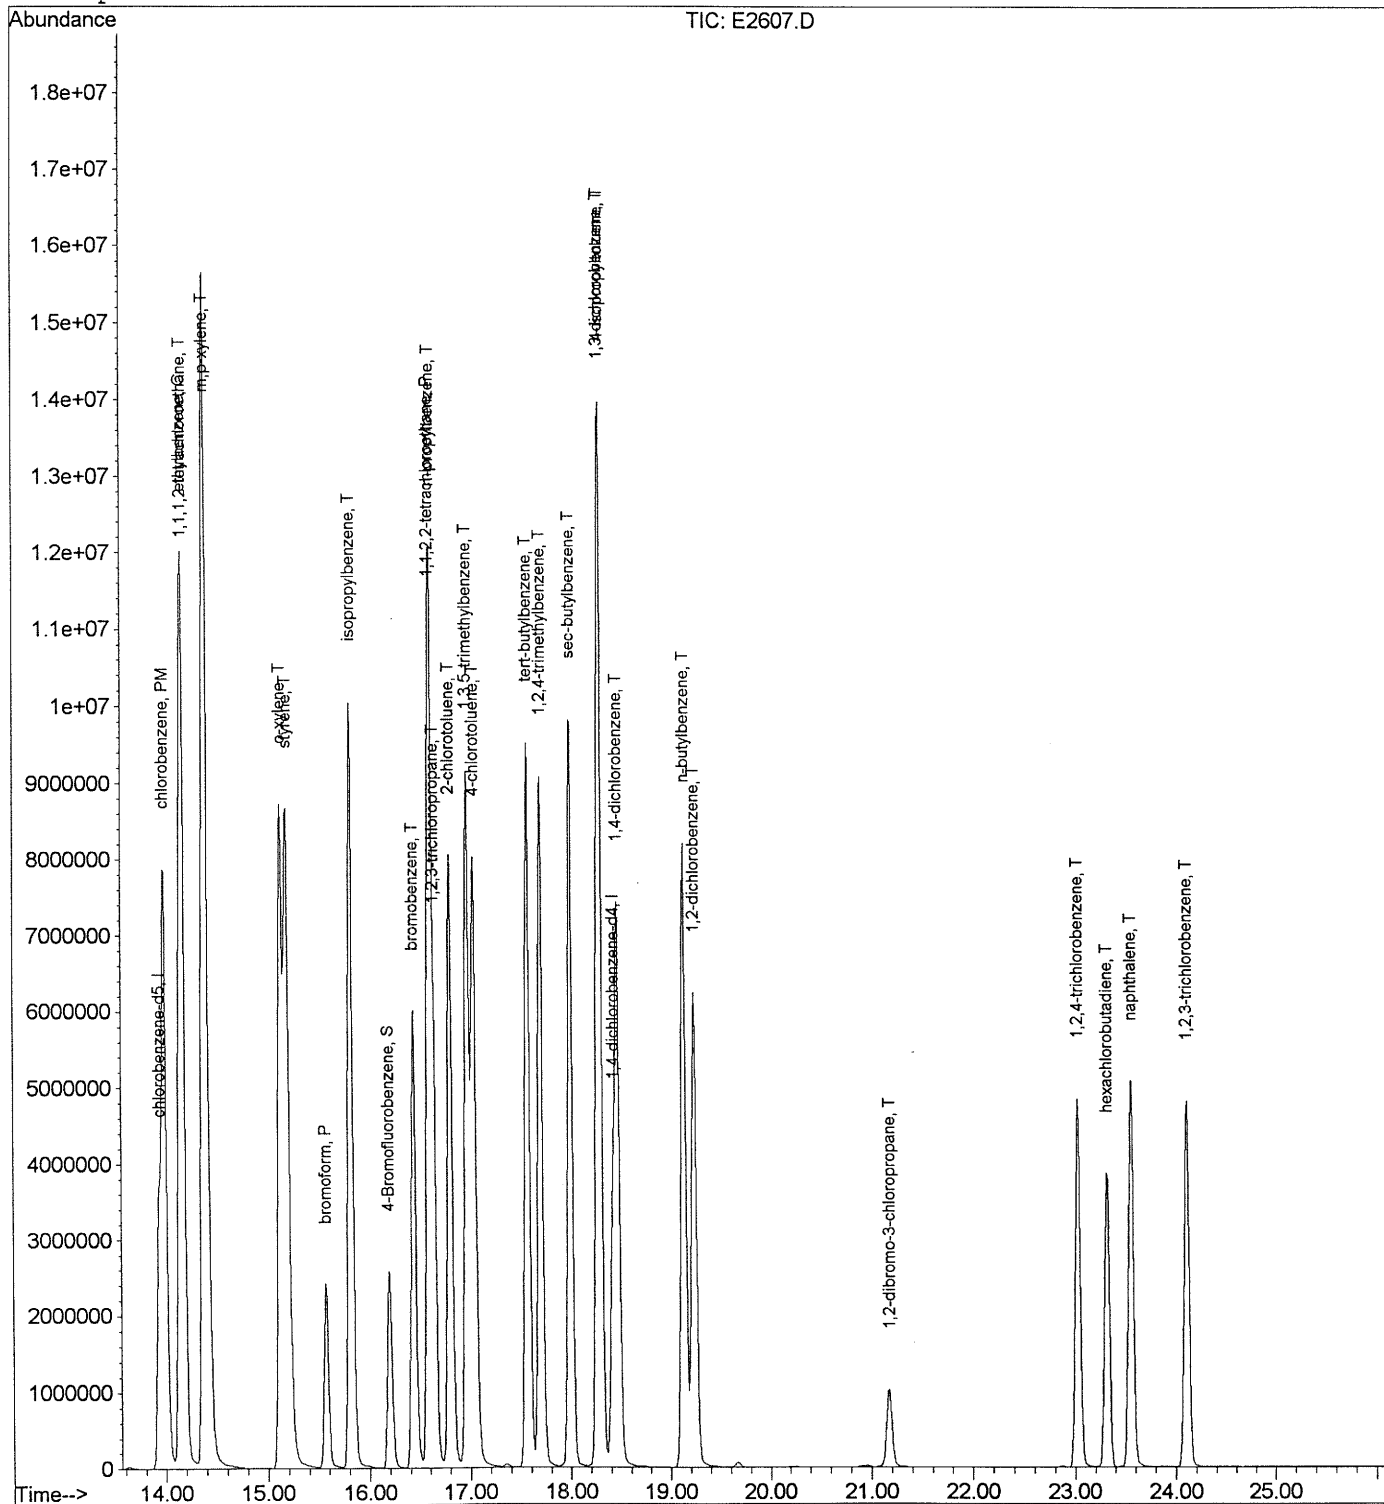

Data File : C:\HPCHEM\1\DATA\040105\E2608.D

Vial: 7

Acq On : 1 Apr 05 11:48 am

Operator: xl

Sample : 200ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:35 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Fri Apr 01 19:18:41 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.60	168	1972453	50.00	ug/Kg	0.00
32) 1,4-difluorobenzene	8.79	114	3836979	50.00	ug/Kg	0.00
49) chlorobenzene-d5	13.94	117	3783293	50.00	ug/Kg	0.00
63) 1,4-dichlorobenzene-d4	18.42	152	1717227	50.00	ug/Kg	0.00

System Monitoring Compounds

29) Dibromofluoromethane	7.47	113	1269470	51.63	ug/Kg	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.26%		
45) toluene-d8	11.26	98	4584156	51.18	ug/Kg	0.00
Spiked Amount 50.000	Range 81 - 120		Recovery =	102.36%		
62) 4-Bromofluorobenzene	16.20	95	1836617	50.33	ug/Kg	0.00
Spiked Amount 50.000	Range 74 - 121		Recovery =	100.66%		

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.67	85	5510540	206.68	ug/Kg	96
3) chloromethane	1.88	50	10060585	199.06	ug/Kg	99
4) vinyl chloride	2.01	62	6680224	219.97	ug/Kg	99
5) bromomethane	2.37	96	852685m	160.34	ug/Kg	96
6) chloroethane	2.49	64	281865	18.70	ug/Kg	96
7) trichlorofluoromethane	2.77	101	4374286	148.01	ug/Kg	99
8) Diethyl Ether	3.23	45	2842090	203.28	ug/Kg	98
10) Acetone	3.77	43	2067971m	196.00	ug/Kg	99
12) 1,1-dichloroethene	3.53	96	3214580	196.97	ug/Kg	96
13) Iodomethane	3.77	142	1332318m	166.36	ug/Kg	88
14) methylene chloride	4.44	84	6199114	205.97	ug/Kg	97
15) Carbon Disulfide	3.81	76	19639380	202.97	ug/Kg	99
16) Acrylonitrile	5.00	53	2215742	255.34	ug/Kg	97
17) tert-Butyl alcohol	4.78	59	7999241	2396.10	ug/Kg	100
18) methyl tert-butyl ether	4.81	73	14887383	218.75	ug/Kg	100
19) trans-1,2-dichloroethene	4.81	96	5260025	195.04	ug/Kg	93
20) 1,1-dichloroethane	5.61	63	10859949	211.67	ug/Kg	100
21) di-isopropyl ether	5.65	45	22342834	218.99	ug/Kg	98
22) Vinyl Acetate	5.71	43	11448453	253.74	ug/Kg	98
23) ethyl tert-butyl ether	6.25	59	18470366	230.28	ug/Kg	99
24) 2-Butanone	6.72	43	3899281	239.75	ug/Kg	99
25) 2,2-dichloropropane	6.53	77	7183778	221.56	ug/Kg	98
26) cis-1,2-dichloroethene	6.62	96	6460338	211.82	ug/Kg	99
27) bromochloromethane	7.03	128	3033060	210.17	ug/Kg	95
28) chloroform	7.19	83	10855926	211.18	ug/Kg	99
30) Tetrahydrofuran	7.06	42	2150829	232.58	ug/Kg	96
31) 1,1,1-trichloroethane	7.37	97	7783477	213.83	ug/Kg	96

(H) = qualifier out of range (m) = manual integration

E2608.D 8260ES6.M

Fri Apr 01 19:53:32 2005

Page 1

000123

Data File : C:\HPCHEM\1\DATA\040105\E2608.D

Vial: 7

Acq On : 1 Apr 05 11:48 am

Operator: xl

Sample : 200ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:35 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Fri Apr 01 19:18:41 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) carbon tetrachloride	7.58	117	6336964m	200.01	ug/Kg	78
34) 1,1-dichloropropene	7.66	75	8777854	185.74	ug/Kg	99
35) benzene	7.98	78	22442529	196.28	ug/Kg	94
36) 1,2-dichloroethane	8.18	62	8071862	199.17	ug/Kg	100
37) tert amyl methyl ether	8.20	73	15409228	222.84	ug/Kg	98
38) trichloroethene	9.14	95	6460085	203.43	ug/Kg	97
39) 1,2-dichloropropane	9.61	63	6842922	210.87	ug/Kg	100
40) dibromomethane	9.82	93	4325076	211.31	ug/Kg	99
41) bromodichloromethane	10.11	83	8798133	216.00	ug/Kg	98
43) 4-Methyl-2-Pentanone	11.20	43	8779643	239.21	ug/Kg	97
44) cis-1,3-dichloropropene	10.91	75	10285688	227.61	ug/Kg	97
47) trans-1,3-dichloropropene	11.97	75	9392927	213.13	ug/Kg	99
48) 1,1,2-trichloroethane	12.28	83	5173377	210.97	ug/Kg	98
50) 2-Hexanone	12.72	43	6076364m	205.30	ug/Kg	99
51) tetrachloroethene	12.32	166	5474120	185.98	ug/Kg	95
52) 1,3-dichloropropane	12.58	76	10417365	210.02	ug/Kg	97
53) dibromochloromethane	12.92	129	6566117	213.78	ug/Kg	100
54) 1,2-dibromoethane	13.12	107	6424989	215.43	ug/Kg	99
55) chlorobenzene	13.99	112	16336667	202.40	ug/Kg	98
56) 1,1,1,2-tetrachloroethane	14.18	131	5159450	194.53	ug/Kg	98
57) ethylbenzene	14.15	91	24513952	173.20	ug/Kg	81
59) o-xylene	15.13	106	9897582	200.70	ug/Kg	89
60) styrene	15.19	104	17906822	209.84	ug/Kg	95
61) bromoform	15.57	173	4320056	223.96	ug/Kg	97
64) isopropylbenzene	15.81	105	24357113	181.61	ug/Kg	84
65) bromobenzene	16.44	156	6505235	203.75	ug/Kg	93
66) 1,1,2,2-tetrachloroethane	16.58	83	8491147	208.79	ug/Kg	100
68) n-propylbenzene	16.61	91	26633412	163.29	ug/Kg	80
69) 2-chlorotoluene	16.80	91	18792452	201.81	ug/Kg	98
70) 4-chlorotoluene	17.04	91	21303485	199.99	ug/Kg	98
71) 1,3,5-trimethylbenzene	16.98	105	20868619	195.78	ug/Kg	94
72) tert-butylbenzene	17.56	91	13034709	201.36	ug/Kg	98
73) 1,2,4-trimethylbenzene	17.69	105	20694181	197.20	ug/Kg	96
74) sec-butylbenzene	17.99	105	24541226	176.45	ug/Kg	90
75) 1,3-dichlorobenzene	18.27	146	10780600	190.64	ug/Kg	99
76) 4-isopropyltoluene	18.29	119	20283291	192.21	ug/Kg	98
77) 1,4-dichlorobenzene	18.47	146	11234544	196.89	ug/Kg	98
78) 1,2-dichlorobenzene	19.23	146	11060653	200.63	ug/Kg	98
79) n-butylbenzene	19.13	91	20828676	210.76	ug/Kg	98
80) 1,2-dibromo-3-chloropropan	21.17	75	1422463	231.58	ug/Kg	92
81) 1,2,4-trichlorobenzene	23.03	180	6049920	201.41	ug/Kg	98

(#) = qualifier out of range (m) = manual integration

Data File : C:\HPCHEM\1\DATA\040105\E2608.D

Vial: 7

Acq On : 1 Apr 05 11:48 am

Operator: xl

Sample : 200ppb 8260s std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 1 19:35 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Fri Apr 01 19:18:41 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
82) hexachlorobutadiene	23.32	225	2911919	192.11	ug/Kg	99
83) naphthalene	23.55	128	18546311	226.17	ug/Kg	100
84) 1,2,3-trichlorobenzene	24.10	180	6031009	196.94	ug/Kg	98

XL 4/1/05


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2608.D
Acq On : 1 Apr 05 11:48 am
Sample : 200ppb 8260s std
Misc : samp 8260_s
MS Integration Params: rteint.p
Quant Time: Apr 1 19:35 19105

Vial: 7
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Fri Apr 01 19:18:41 2005
Response via : Initial Calibration

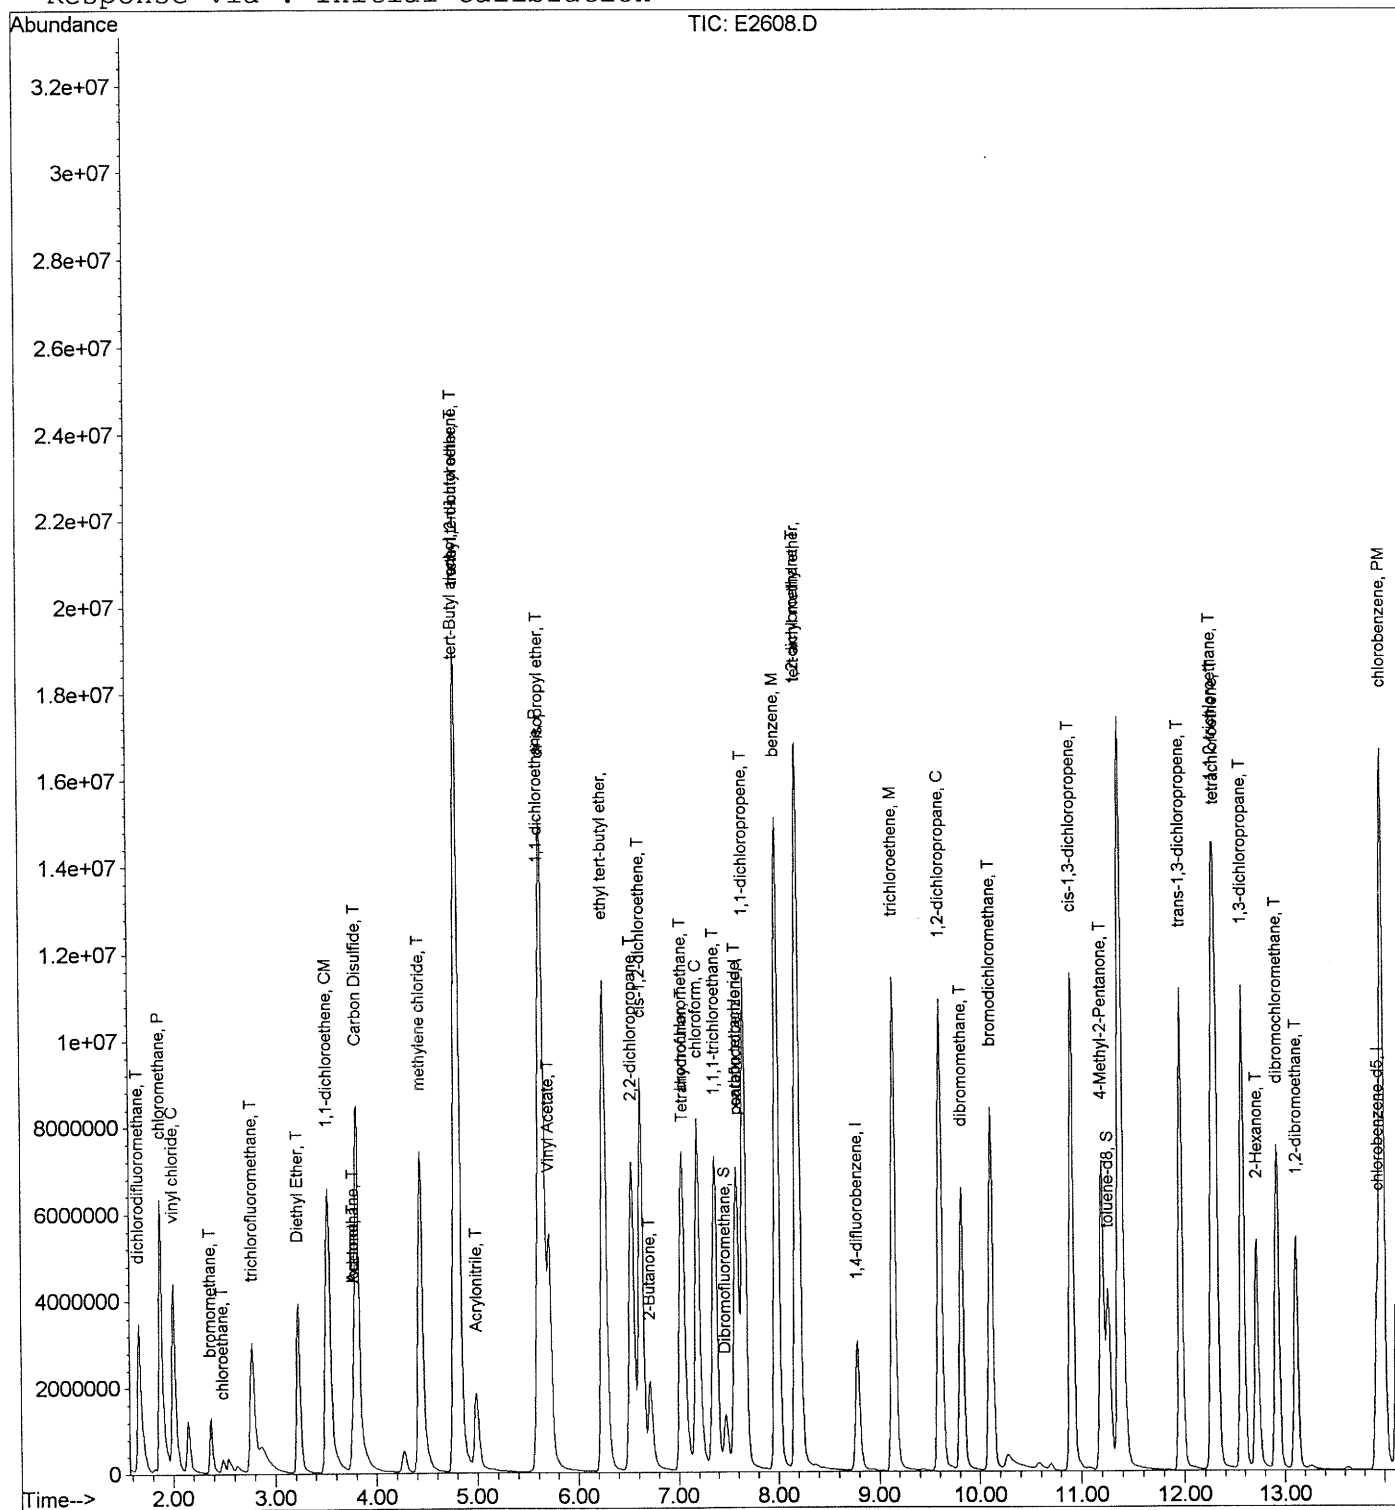


Quantitation Report

Data File : C:\HPCHEM\1\DATA\040105\E2608.D
 Acq On : 1 Apr 05 11:48 am
 Sample : 200ppb 8260s std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 1 19:35 19105

Vial: 7
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\040105\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Fri Apr 01 19:18:41 2005
 Response via : Initial Calibration

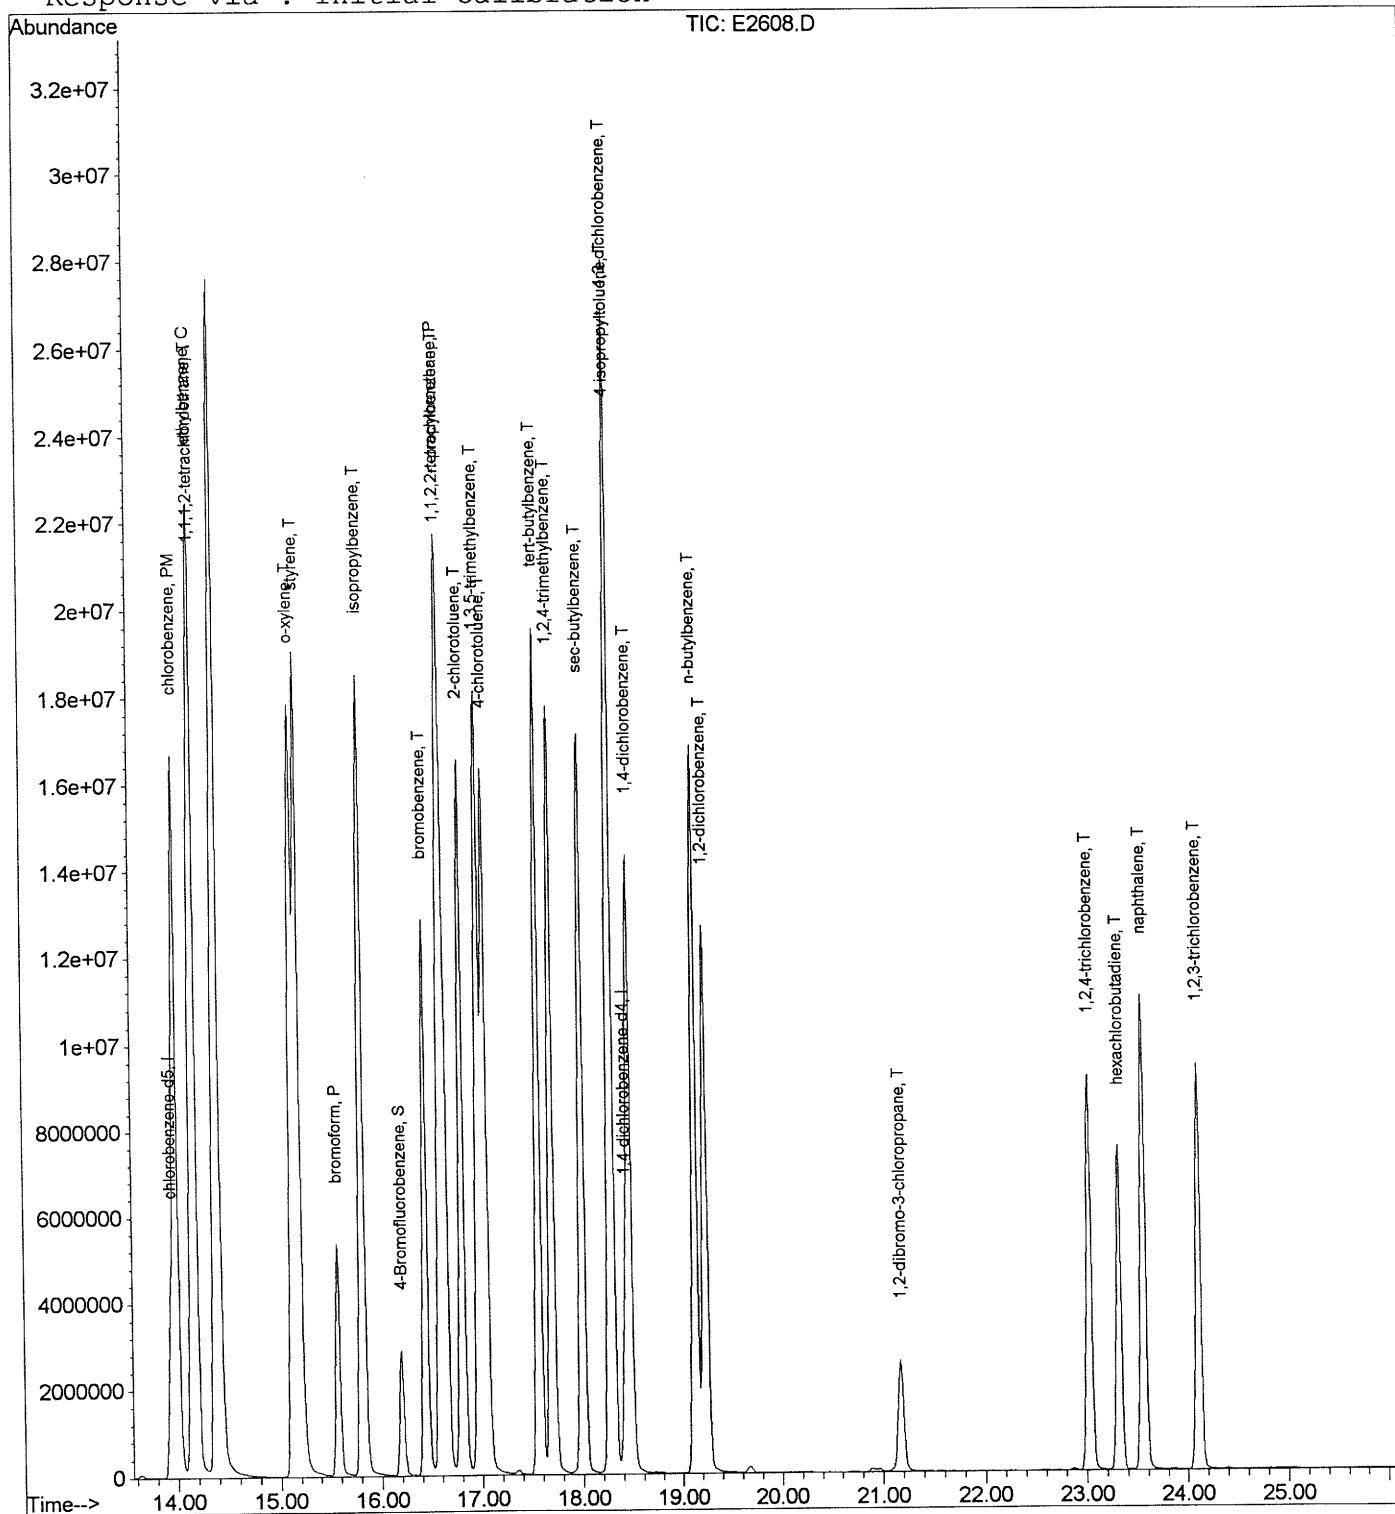

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: Toxikon Corporation Contract: _____
 Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____
 Instrument ID: E Calibration Date: 04/29/05 Time: 9:36
 Lab File E2775.D Init. Calib. DATE(s): 04/01/05 04/01/05
 EPA Sample No. (VSTD050##): ZZZZZDL Init. Calib. Times: 9:32 11:48
 Heated Purge: (Y/N) Y
 GC Column: RTX-624 ID 0.3 (mm)

COMPOUND	RRF	RRF50	MIN RRF	%D	MAX %D
1,1,1,2-Tetrachloroethane	0.348	0.36		-5.1	20.0
1,1,1-Trichloroethane	0.935	0.990		-6.7	20.0
1,1,2,2-Tetrachloroethane	1.195	1.148	0.300	4.2	20.0
1,1,2-Trichloroethane	0.323	0.328		-2.4	20.0
1,1-Dichloroethane	1.315	1.342	0.100	-2.7	20.0
1,1-Dichloroethene	0.412	0.481		-16.9	20.0
1,1-Dichloropropene	0.607	0.624		-3.0	20.0
1,2,3-Trichlorobenzene	0.889	0.972		-11.6	20.0
1,2,3-Trichloropropane	0.287	0.284		1.6	20.0
1,2,4-Trichlorobenzene	0.876	1.022		-19.1	20.0
1,2,4-Trimethylbenzene	3.047	3.067		-1.2	20.0
1,2-Dibromo-3-chloropropane	0.176	0.173		-2.0	20.0
1,2-Dibromoethane	0.400	0.405		-2.3	20.0
1,2-Dichlorobenzene	1.606	1.623		-1.3	20.0
1,2-Dichloroethane	0.528	0.547		-3.4	20.0
1,2-Dichloropropane	0.427	0.423		0.2	20.0
1,3,5-Trimethylbenzene	3.090	3.135		-1.8	20.0
1,3-Dichlorobenzene	1.631	1.684		-2.8	20.0
1,3-Dichloropropane	0.620	0.650		1.4	20.0
1,4-Dichlorobenzene	1.656	1.694		-1.7	20.0
2,2-Dichloropropane	0.840	0.954		-15.0	20.0
2-Butanone	0.429	0.414		3.4	20.0
2-Chloroethyl vinyl ether	0.004	0.003		14.1	20.0
2-Chlorotoluene	2.716	2.687		0.7	20.0
2-Hexanone	0.359	0.359		-1.8	20.0
4-Chlorotoluene	3.101	3.024		2.7	20.0
4-Isopropyltoluene	3.049	3.183		-5.1	20.0
4-Methyl-2-pentanone	0.497	0.499		0.7	20.0
Acetone	0.268	0.258		10.5	20.0
Acrylonitrile	0.232	0.214		6.2	20.0
Benzene	1.221	1.550		-4.5	20.0
Bromobenzene	0.933	0.929		0.4	20.0
Bromochloromethane	0.411	0.395		-6.8	20.0
Bromodichloromethane	0.539	0.550		-3.9	20.0
Bromoform	0.261	0.282	0.100	-11.1	20.0

All other compounds must meet a minimum RRF of 0.010.

FORM VII

OLM03.0

HB

000128

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: Toxikon Corporation Contract: _____
 Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209
 Instrument ID: E Calibration Date: 04/29/05 Time: 9:36
 Lab File E2775.D Init. Calib. DATE(s): 04/01/05 04/01/05
 EPA Sample No. (VSTD050##): ZZZZZDL Init. Calib. Times: 9:32 11:48
 Heated Purge: (Y/N) Y
 GC Column: RTX-624 ID 0.3 (mm)

COMPOUND	RRF	RRF5	MIN RRF	%D	MAX %D
Bromomethane	0.242	0.198		27.8	20.0
Carbon disulfide	2.460	2.388		1.4	20.0
Carbon tetrachloride	0.458	0.456		10.3	20.0
Chlorobenzene	1.070	1.080	0.300	-0.5	20.0
Chloroethane	0.382	0.417		-6.2	20.0
Chloroform	1.318	1.382		-5.5	20.0
Chloromethane	1.280	1.226	0.100	4.9	20.0
cis-1,2-Dichloroethene	0.782	0.804		-3.2	20.0
cis-1,3-Dichloropropene	0.605	0.649		-10.7	20.0
Dibromochloromethane	0.539	0.424		-5.2	20.0
Dibromomethane	0.270	0.280		-4.7	20.0
Dichlorodifluoromethane	0.680	0.728		-6.3	20.0
Ethylbenzene	1.821	1.894		-4.0	20.0
Hexachlorobutadiene	0.438	0.489		-13.5	20.0
Iodomethane	0.140	0.170		-25.2	20.0
Isopropylbenzene	3.833	3.801		0.6	20.0
Methylene chloride	0.774	0.766		1.9	20.0
n-Butylbenzene	2.098	3.113		-8.8	20.0
n-Propylbenzene	4.574	4.631		-1.3	20.0
Naphthalene	2.450	2.646		-12.1	20.0
sec-Butylbenzene	3.954	3.983		-1.3	20.0
Styrene	1.139	1.165		-3.8	20.0
tert-Butylbenzene	1.888	1.809		3.7	20.0
Tetrachloroethene	0.384	0.426		-10.0	20.0
Tetrahydrofuran	0.242	0.233		8.2	20.0
Toluene	0.926	0.965		-4.4	20.0
trans-1,2-Dichloroethene	0.680	0.720		-6.0	20.0
trans-1,3-Dichloropropene	0.533	0.579		-13.3	20.0
Trichloroethene	0.415	0.426		-3.2	20.0
Trichlorofluoromethane	0.710	0.792		-10.7	20.0
Vinyl acetate	1.205	1.270		-7.6	20.0
Vinyl chloride	0.785	0.779		0.2	20.0
Xylenes, Total	1.319	1.320		-2.2	20.0

All other compounds must meet a minimum RRF of 0.010.

FORM VII

OLM03.0

000129

7A
VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: Toxikon Corporation Contract: _____
Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209
Instrument ID: E Calibration Date: 04/29/05 Time: 9:36
Lab File E2775.D Init. Calib. DATE(s): 04/01/05 04/01/05
EPA Sample No. (VSTD050##): ZZZZZDL Init. Calib. Times: 9:32 11:48
Heated Purge: (Y/N) Y
GC Column: RTX-624 ID 0.3 (mm)

COMPOUND	RRF	RRF50	MIN RRF	%D	MAX %D
4-Bromofluorobenzene	0.483	0.493		-2.4	20.0
Dibromofluoromethane	0.680	0.630		-1.0	20.0
Toluene-d8	1.172	1.170		0.8	20.0

All other compounds must meet a minimum RRF of 0.010.

FORM VII

OLM03.0

000130

Continuing Calibration Report inst e

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

Continuing Calibration File: E2775.D

Min. RRF : 0.000 Min. Rel. Area : 50%
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%
1 I	pentafluorobenzene	1.000	1.000	0.0	101
2 T	dichlorodifluoromethane	0.684	0.728	-6.3	111
3 P	chloromethane	1.290	1.226	4.9	99
4 C	vinyl chloride	0.781	0.779	0.2	104
5 T	bromomethane	0.274	0.198	27.8#	101
6 T	chloroethane	0.392	0.417	-6.2	106
7 T	trichlorofluoromethane	0.716	0.792	-10.7	109
8 T	Diethyl Ether	0.360	0.289	19.8	83
9 T	Acrolein	0.041	0.036	12.1	89
10 T	Acetone	0.288	0.258	10.5	98
11	Iso-propyl alcohol	0.000	0.000	0.0	77
12 CM	1,1-dichloroethene	0.412	0.481	-16.9	116
13 T	Iodomethane	0.136	0.170	-25.2#	125
14 T	methylene chloride	0.781	0.766	1.9	103
15 T	Carbon Disulfide	2.423	2.388	1.4	98
16 T	Acrylonitrile	0.228	0.214	6.2	95
17	tert-Butyl alcohol	0.087	0.084	4.3	98
18 T	methyl tert-butyl ether	1.749	1.723	1.5	99
19 T	trans-1,2-dichloroethene	0.679	0.720	-6.0	107
20 P	1,1-dichloroethane	1.307	1.342	-2.7	104
21 T	di-isopropyl ether	2.606	2.475	5.0	96
22 T	Vinyl Acetate	1.180	1.270	-7.6	110
23	ethyl tert-butyl ether	2.061	2.004	2.8	98
24 T	2-Butanone	0.428	0.414	3.4	96
25 T	2,2-dichloropropane	0.830	0.954	-15.0	118
26 T	cis-1,2-dichloroethene	0.779	0.804	-3.2	105
27 T	bromochloromethane	0.369	0.395	-6.8	108
28 C	chloroform	1.310	1.382	-5.5	108
29 S	Dibromofluoromethane	0.624	0.630	-1.0	101
30 T	Tetrahydrofuran	0.253	0.233	8.2	99
31 T	1,1,1-trichloroethane	0.928	0.990	-6.7	108
32 I	1,4-difluorobenzene	1.000	1.000	0.0	100
33 T	carbon tetrachloride	0.509	0.456	10.3	107
34 T	1,1-dichloropropene	0.606	0.624	-3.0	104
35 M	benzene	1.483	1.550	-4.5	104
36 T	1,2-dichloroethane	0.529	0.547	-3.4	103
37	tert amyl methyl ether	0.910	0.917	-0.8	100
38 M	trichloroethene	0.412	0.426	-3.2	102
39 C	1,2-dichloropropane	0.424	0.423	0.2	100
40 T	dibromomethane	0.268	0.280	-4.7	103
41 T	bromodichloromethane	0.529	0.550	-3.9	103
42 T	2-Chloroethyl vinyl ether	0.004	0.003	14.1	136

(#) = Out of Range

E2775.D 8260ES6.M Fri Apr 29 10:23:12 2005

000131

Page 1

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

Continuing Calibration File: E2775.D

Min. RRF : 0.000 Min. Rel. Area : 50%
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%
43 T	4-Methyl-2-Pentanone	0.503	0.499	0.7	100
44 T	cis-1,3-dichloropropene	0.586	0.649	-10.7	107
45 S	toluene-d8	1.170	1.167	0.3	99
46 CM	toluene	0.924	0.965	-4.4	105
47 T	trans-1,3-dichloropropene	0.511	0.579	-13.3	108
48 T	1,1,2-trichloroethane	0.320	0.328	-2.4	100
49 I	chlorobenzene-d5	1.000	1.000	0.0	103
50 T	2-Hexanone	0.353	0.359	-1.8	100
51 T	tetrachloroethene	0.387	0.426	-10.0	115
52 T	1,3-dichloropropane	0.659	0.650	1.4	101
53 T	dibromochloromethane	0.403	0.424	-5.2	107
54 T	1,2-dibromoethane	0.396	0.405	-2.3	105
55 PM	chlorobenzene	1.074	1.080	-0.5	106
56 T	1,1,1,2-tetrachloroethane	0.346	0.364	-5.1	108
57 C	ethylbenzene	1.821	1.894	-4.0	105
58 T	m,p-xylene	0.668	0.682	-2.2	105
59 T	o-xylene	0.648	0.662	-2.2	106
60 T	styrene	1.123	1.165	-3.8	106
61 P	bromoform	0.254	0.282	-11.1	113
62 S	4-Bromofluorobenzene	0.482	0.493	-2.3	106
63 I	1,4-dichlorobenzene-d4	1.000	1.000	0.0	109
64 T	isopropylbenzene	3.824	3.801	0.6	107
65 T	bromobenzene	0.933	0.929	0.4	109
66 P	1,1,2,2-tetrachloroethane	1.198	1.148	4.2	105
67 T	1,2,3-trichloropropane	0.288	0.284	1.6	106
68 T	n-propylbenzene	4.571	4.631	-1.3	107
69 T	2-chlorotoluene	2.708	2.687	0.7	109
70 T	4-chlorotoluene	3.107	3.024	2.7	108
71 T	1,3,5-trimethylbenzene	3.078	3.135	-1.8	111
72 T	tert-butylbenzene	1.878	1.809	3.7	106
73 T	1,2,4-trimethylbenzene	3.030	3.067	-1.2	111
74 T	sec-butylbenzene	3.931	3.983	-1.3	108
75 T	1,3-dichlorobenzene	1.637	1.684	-2.8	112
76 T	4-isopropyltoluene	3.029	3.183	-5.1	113
77 T	1,4-dichlorobenzene	1.666	1.694	-1.7	112
78 T	1,2-dichlorobenzene	1.602	1.623	-1.3	110
79 T	n-butylbenzene	2.862	3.113	-8.8	117
80 T	1,2-dibromo-3-chloropropane	0.169	0.173	-2.0	107
81 T	1,2,4-trichlorobenzene	0.858	1.022	-19.1	125
82 T	hexachlorobutadiene	0.431	0.489	-13.5	122
83 T	naphthalene	2.361	2.646	-12.1	113

(#) = Out of Range

Continuing Calibration Report inst e

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Mon Apr 04 10:16:13 2005
Response via : Initial Calibration

Continuing Calibration File: E2775.D

Min. RRF : 0.000 Min. Rel. Area : 50%
Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%
84 T	1,2,3-trichlorobenzene	0.871	0.972	-11.6	118

Yc 5/2/05

Data File : C:\HPCHEM\1\DATA\042905\E2775.D

Vial: 2

Acq On : 29 Apr 05 9:36 am

Operator: xl

Sample : 50ppb 8260 std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 29 10:21 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Apr 04 10:16:13 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.61	168	1944140	50.00	ug/Kg	0.00
32) 1,4-difluorobenzene	8.80	114	3600616	50.00	ug/Kg	0.02
49) chlorobenzene-d5	13.94	117	3582408	50.00	ug/Kg	0.02
63) 1,4-dichlorobenzene-d4	18.44	152	1735466	50.00	ug/Kg	0.02

System Monitoring Compounds

29) Dibromofluoromethane	7.49	113	1225201	50.49	ug/Kg	0.02
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.98%
45) toluene-d8	11.28	98	4200729	49.87	ug/Kg	0.02
Spiked Amount	50.000	Range	81 - 120	Recovery	=	99.74%
62) 4-Bromofluorobenzene	16.21	95	1767643	51.17	ug/Kg	0.02
Spiked Amount	50.000	Range	74 - 121	Recovery	=	102.34%

Target Compounds

					Qvalue
2) dichlorodifluoromethane	1.68	85	1414637	53.17	ug/Kg 97
3) chloromethane	1.90	50	2384142	47.53	ug/Kg 100
4) vinyl chloride	2.01	62	1515252	49.89	ug/Kg 99
5) bromomethane	2.39	96	384030m	46.83	ug/Kg 98
6) chloroethane	2.53	64	810327	53.12	ug/Kg 100
7) trichlorofluoromethane	2.82	101	1540489	55.36	ug/Kg 99
8) Diethyl Ether	3.25	45	561721m	40.11	ug/Kg 97
9) Acrolein	4.82	56	347627m	219.83	ug/Kg 55
10) Acetone	3.79	43	500897	50.86	ug/Kg 98
12) 1,1-dichloroethene	3.56	96	934911	58.43	ug/Kg 96
13) Iodomethane	3.80	142	330961	62.60	ug/Kg 94
14) methylene chloride	4.45	84	1490098	49.07	ug/Kg 97
15) Carbon Disulfide	3.85	76	4643126	49.28	ug/Kg 99
16) Acrylonitrile	5.00	53	416172	46.89	ug/Kg 99
17) tert-Butyl alcohol	4.76	59	1624051	478.36	ug/Kg 100
18) methyl tert-butyl ether	4.82	73	3349997	49.25	ug/Kg 100
19) trans-1,2-dichloroethene	4.83	96	1399250	52.99	ug/Kg 98
20) 1,1-dichloroethane	5.62	63	2608614	51.34	ug/Kg 98
21) di-isopropyl ether	5.65	45	4812127	47.48	ug/Kg 99
22) Vinyl Acetate	5.73	43	2469496	53.81	ug/Kg 100
23) ethyl tert-butyl ether	6.27	59	3896597	48.61	ug/Kg 98
24) 2-Butanone	6.73	43	804187	48.32	ug/Kg 99
25) 2,2-dichloropropane	6.55	77	1854908	57.50	ug/Kg 99
26) cis-1,2-dichloroethene	6.64	96	1562827	51.62	ug/Kg 100
27) bromochloromethane	7.05	128	767167	53.40	ug/Kg 95
28) chloroform	7.21	83	2686171	52.74	ug/Kg 100
30) Tetrahydrofuran	7.08	42	452225	45.89	ug/Kg 98

(#)=qualifier out of range (m)=manual integration

E2775.D 8260ES6.M

Fri Apr 29 10:22:05 2005

xl 5/10

Page 1

000134

Data File : C:\HPCHEM\1\DATA\042905\E2775.D

Vial: 2

Acq On : 29 Apr 05 9:36 am

Operator: xl

Sample : 50ppb 8260 std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 29 10:21 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Apr 04 10:16:13 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) 1,1,1-trichloroethane	7.38	97	1924407	53.34	ug/Kg	96
33) carbon tetrachloride	7.60	117	1643245	52.36	ug/Kg	82
34) 1,1-dichloropropene	7.67	75	2248579	51.52	ug/Kg	100
35) benzene	8.00	78	5580194	52.26	ug/Kg	99
36) 1,2-dichloroethane	8.19	62	1968363	51.71	ug/Kg	99
37) tert amyl methyl ether	8.21	73	3301087	50.38	ug/Kg	99
38) trichloroethene	9.16	95	1533320	51.62	ug/Kg	99
39) 1,2-dichloropropane	9.62	63	1522831	49.91	ug/Kg	100
40) dibromomethane	9.83	93	1008775	52.36	ug/Kg	94
41) bromodichloromethane	10.13	83	1979406	51.93	ug/Kg	98
42) 2-Chloroethyl vinyl ether	10.72	63	12260m	76.25	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.21	43	1798356	49.65	ug/Kg	98
44) cis-1,3-dichloropropene	10.92	75	2336686	55.33	ug/Kg	100
46) toluene	11.39	92	3475213	52.21	ug/Kg	98
47) trans-1,3-dichloropropene	11.99	75	2085781	56.64	ug/Kg	99
48) 1,1,2-trichloroethane	12.30	83	1179483	51.22	ug/Kg	98
50) 2-Hexanone	12.73	43	1285087	50.88	ug/Kg	99
51) tetrachloroethene	12.32	166	1524405	54.99	ug/Kg	98
52) 1,3-dichloropropane	12.59	76	2328264	49.32	ug/Kg	98
53) dibromochloromethane	12.94	129	1519440	52.62	ug/Kg	100
54) 1,2-dibromoethane	13.13	107	1451264	51.14	ug/Kg	98
55) chlorobenzene	14.00	112	3869580	50.27	ug/Kg	97
56) 1,1,1,2-tetrachloroethane	14.19	131	1302675	52.53	ug/Kg	94
57) ethylbenzene	14.16	91	6785935	52.02	ug/Kg	99
58) m,p-xylene	14.39	106	4887454	102.18	ug/Kg	96
59) o-xylene	15.14	106	2372852	51.12	ug/Kg	99
60) styrene	15.20	104	4174136	51.88	ug/Kg	95
61) bromoform	15.58	173	1009899	55.57	ug/Kg	97
64) isopropylbenzene	15.83	105	6596248	49.70	ug/Kg	99
65) bromobenzene	16.45	156	1613044	49.80	ug/Kg	99
66) 1,1,2,2-tetrachloroethane	16.60	83	1991846	47.90	ug/Kg	97
67) 1,2,3-trichloropropane	16.66	110	492459	49.21	ug/Kg	96
68) n-propylbenzene	16.62	91	8036880	50.65	ug/Kg	98
69) 2-chlorotoluene	16.82	91	4663894m	49.63	ug/Kg	97
70) 4-chlorotoluene	17.05	91	5247404	48.66	ug/Kg	99
71) 1,3,5-trimethylbenzene	16.98	105	5439862	50.92	ug/Kg	99
72) tert-butylbenzene	17.58	91	3140314	48.17	ug/Kg	95
73) 1,2,4-trimethylbenzene	17.70	105	5322148	50.61	ug/Kg	100
74) sec-butylbenzene	18.01	105	6912972	50.67	ug/Kg	98
75) 1,3-dichlorobenzene	18.28	146	2922311	51.42	ug/Kg	99
76) 4-isopropyltoluene	18.31	119	5524250	52.55	ug/Kg	98

(#)=qualifier out of range (m)=manual integration

E2775.D 8260ES6.M Fri Apr 29 10:22:06 2005

Page 2

000135

Data File : C:\HPCHEM\1\DATA\042905\E2775.D

Vial: 2

Acq On : 29 Apr 05 9:36 am

Operator: xl

Sample : 50ppb 8260 std

Inst : inst e

Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 29 10:21 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Apr 04 10:16:13 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) 1,4-dichlorobenzene	18.48	146	2939096	50.84	ug/Kg	98
78) 1,2-dichlorobenzene	19.25	146	2817445	50.67	ug/Kg	99
79) n-butylbenzene	19.14	91	5401908	54.38	ug/Kg	98
80) 1,2-dibromo-3-chloropropan	21.19	75	299557	51.01	ug/Kg	99
81) 1,2,4-trichlorobenzene	23.05	180	1773425m	59.55	ug/Kg	99
82) hexachlorobutadiene	23.33	225	848578	56.77	ug/Kg	100
83) naphthalene	23.57	128	4592459	56.04	ug/Kg	100
84) 1,2,3-trichlorobenzene	24.12	180	1686487	55.80	ug/Kg	99

XC H/MS


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2775.D
 Acq On : 29 Apr 05 9:36 am
 Sample : 50ppb 8260 std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 29 10:21 19105

Vial: 2
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042505\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

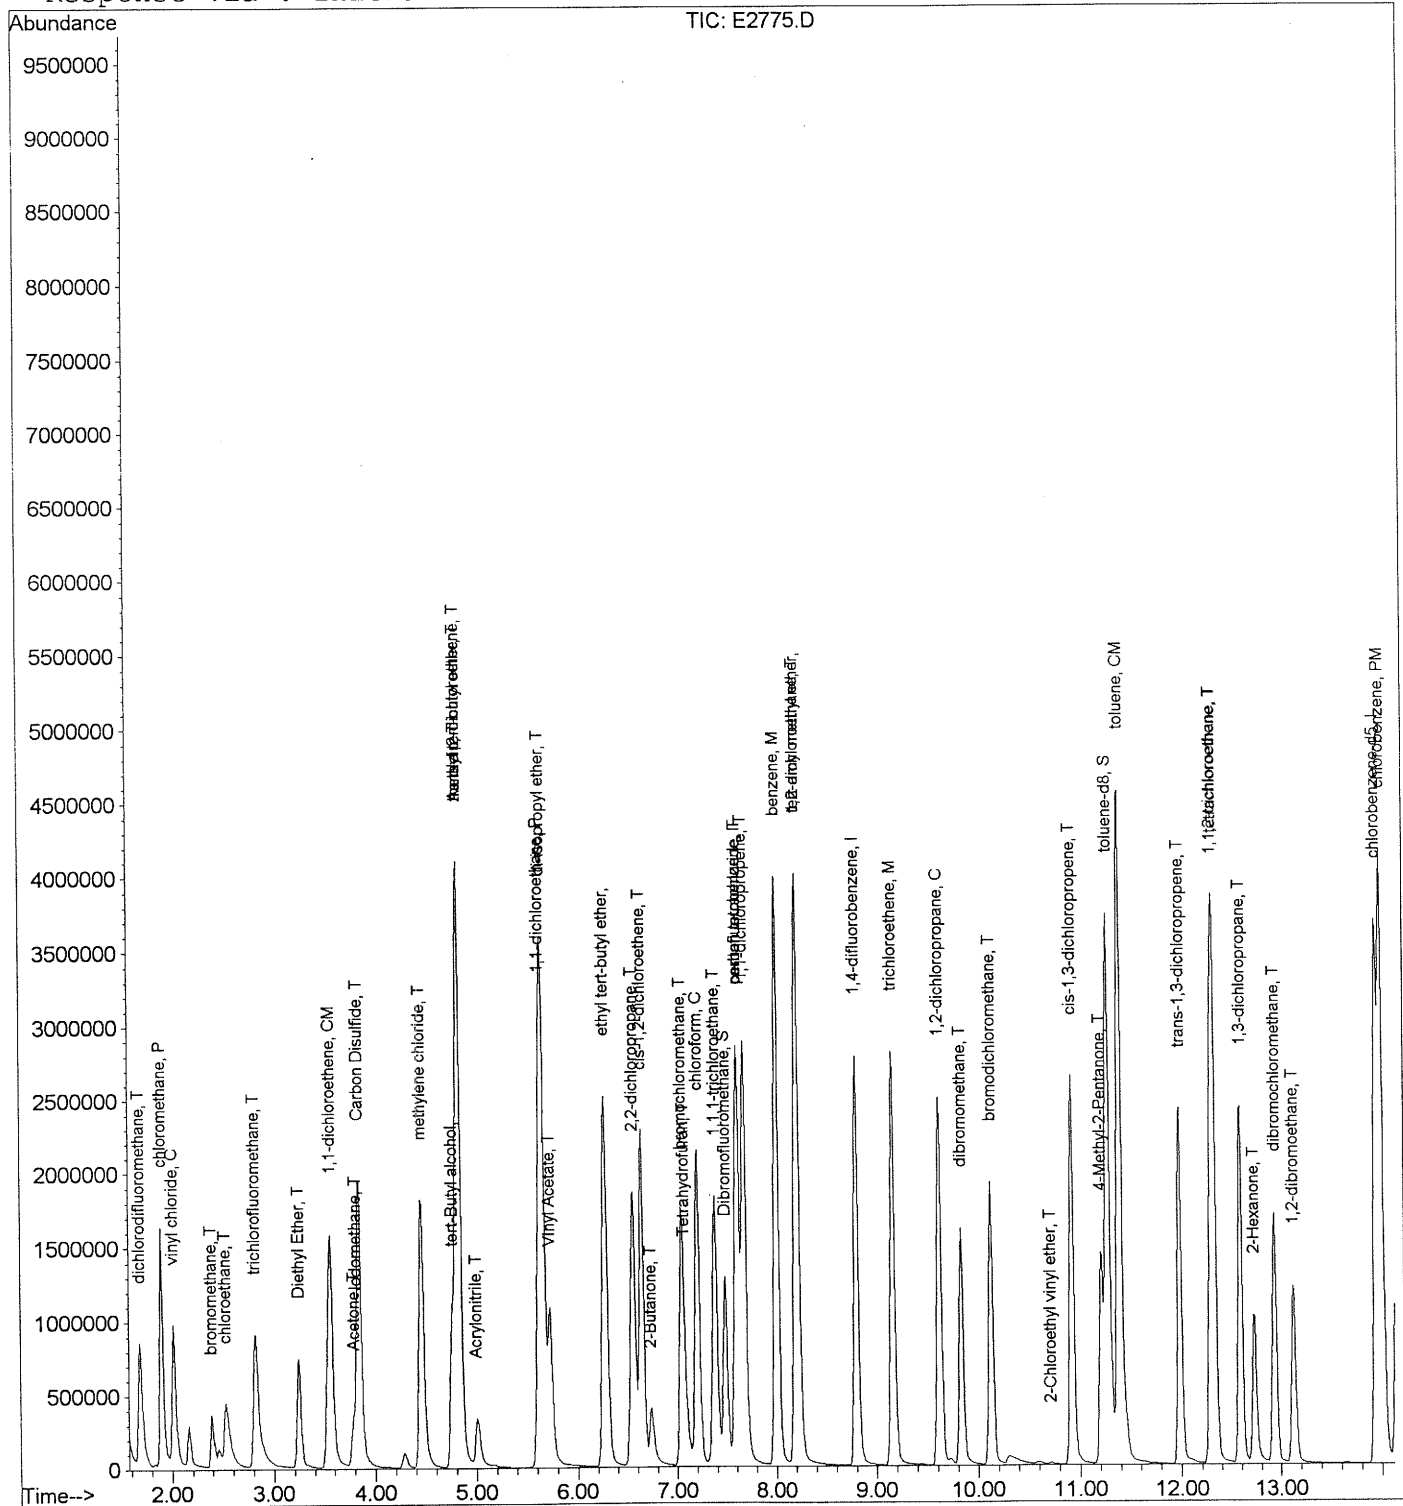


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2775.D
 Acq On : 29 Apr 05 9:36 am
 Sample : 50ppb 8260 std
 Misc : samp 8260_s
 MS Integration Params: rteint.p
 Quant Time: Apr 29 10:21 19105

Vial: 2
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042505\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

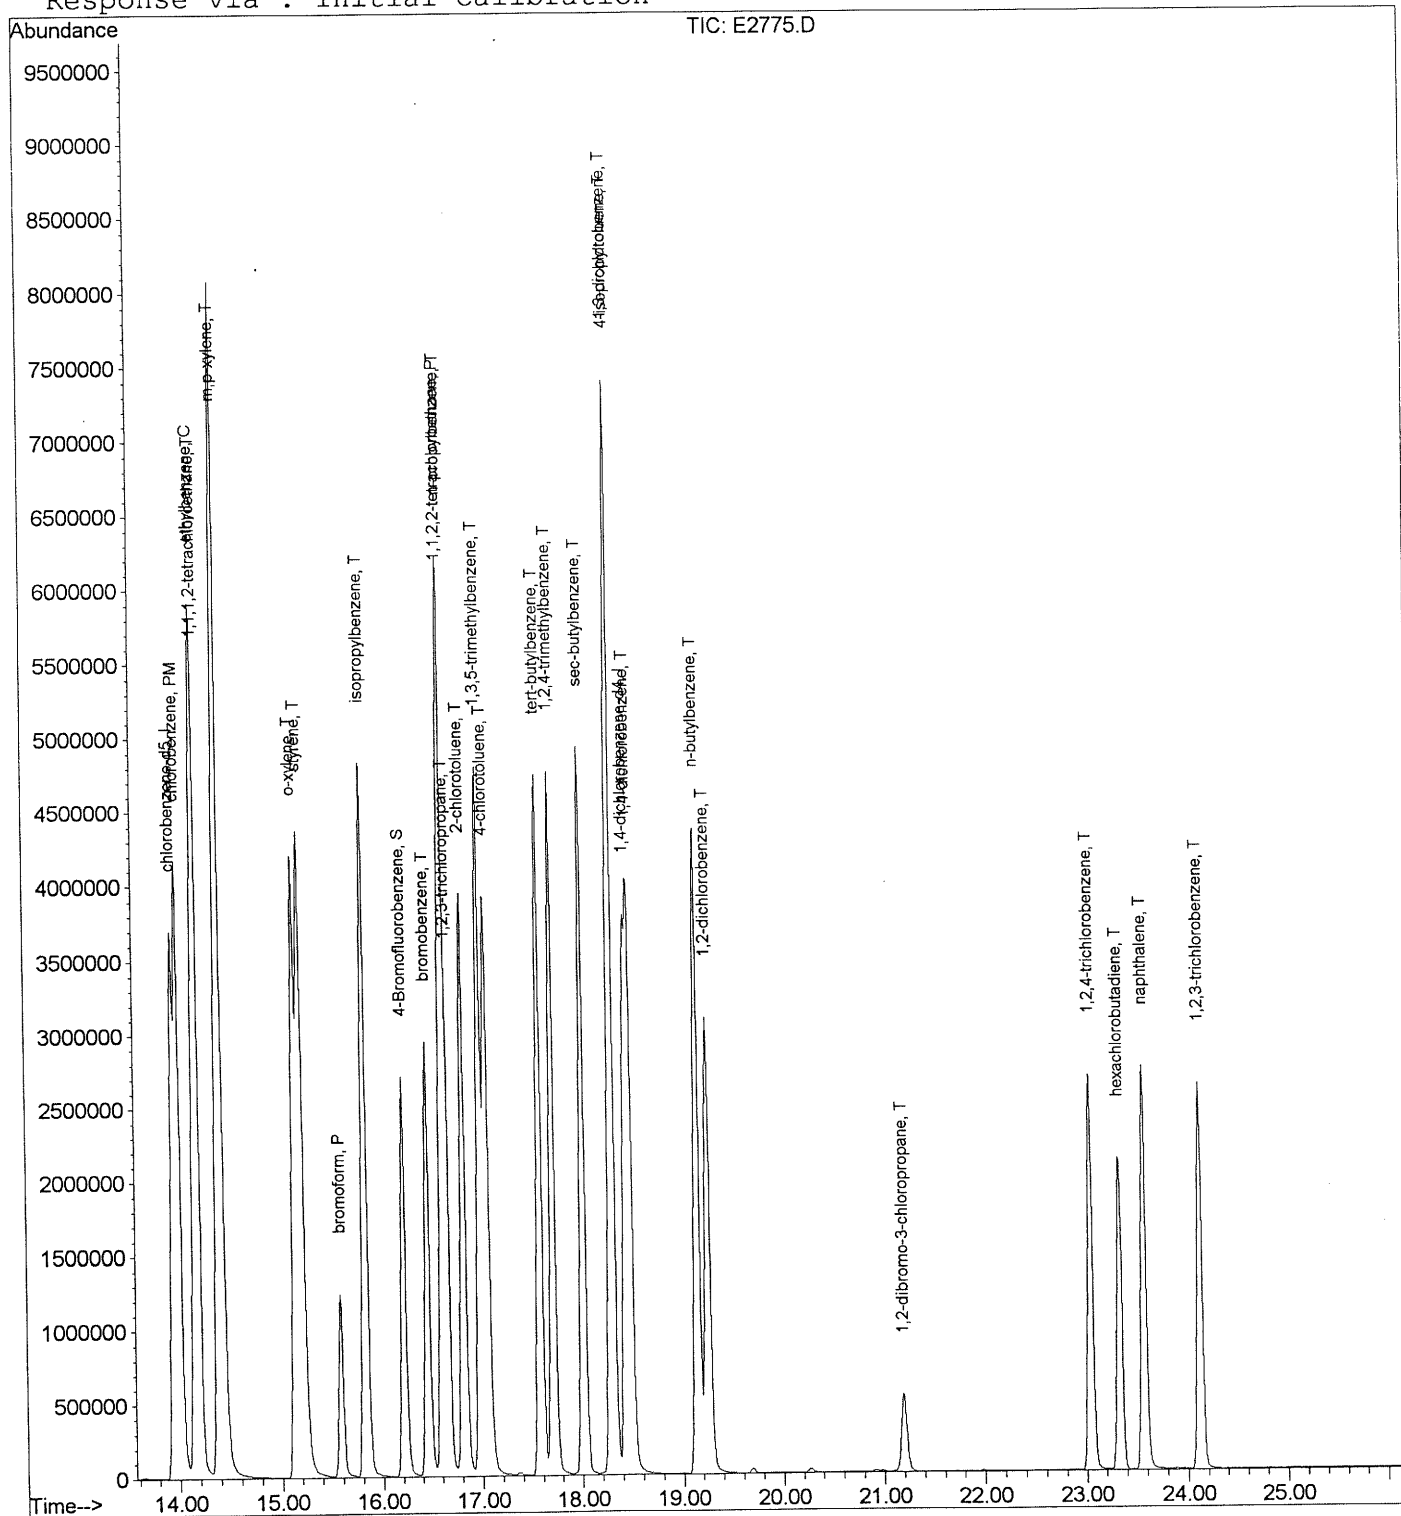

5A

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Toxikon Corporation Contract: _____
 Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209
 Lab File ID: C:\HPCHE BFB Injection Date: 4/29/2005
 Instrument ID: E BFB Injection Time: 8:36
 GC Column: RTX-624 ID: 0.32 (mm) Heated Purge: (Y/N) N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	8.0 - 40.0% of mass 95	21.6
75	30.0 - 66.0% of mass 95	49.5
95	Base peak, 100% relative abundance	100.0
96	5.0 - 9.0% of mass 95	7.0
173	Less than 2.0% of mass 174	0.1 (0.2)1
174	50.0 - 120.0% of mass 95	73.6
175	5.0 - 9.0% of mass 174	5.2 (7.0)1
176	93.0 - 101.0% of mass 174	71.7 (97.4)1
177	5.0 - 9.0% of mass 176	4.7 (6.5)2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS AND STANDARDS:

	EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
01	vstd050	vstd050	E2775.D	04/29/05	9:36
02	MBLK042905	MBLK042905	E2777.D	04/29/05	10:51
03	MW-9 B (5-7)	0504209-01A	E2781.D	04/29/05	13:16
04	MW-9 C (5-7)	0504209-02A	E2782.D	04/29/05	13:49
05	MW-2 B (0-5)	0504209-03A	E2783.D	04/29/05	14:23
06	MW-2 B (43-45)	0504209-04A	E2784.D	04/29/05	14:57
07	MW-2 B (43-45)MS	0504209-04A	E2785.D	04/29/05	15:31
08	MW-2 B (43-45)MSD	0504209-04A	E2786.D	04/29/05	16:04

BFB

Data File : C:\HPCHEM\1\DATA\042905\E2773.D

Vial: 1

Acq On : 29 Apr 05 8:36 am

Operator: xl

Sample : 50ng bfb std

Inst : inst e


Misc : samp 8260_s

Multiplr: 1.00

MS Integration Params: rteint.p

Method : C:\HPCHEM\1\DATA\042905\BFB_E.M (RTE Integrator)

Title :

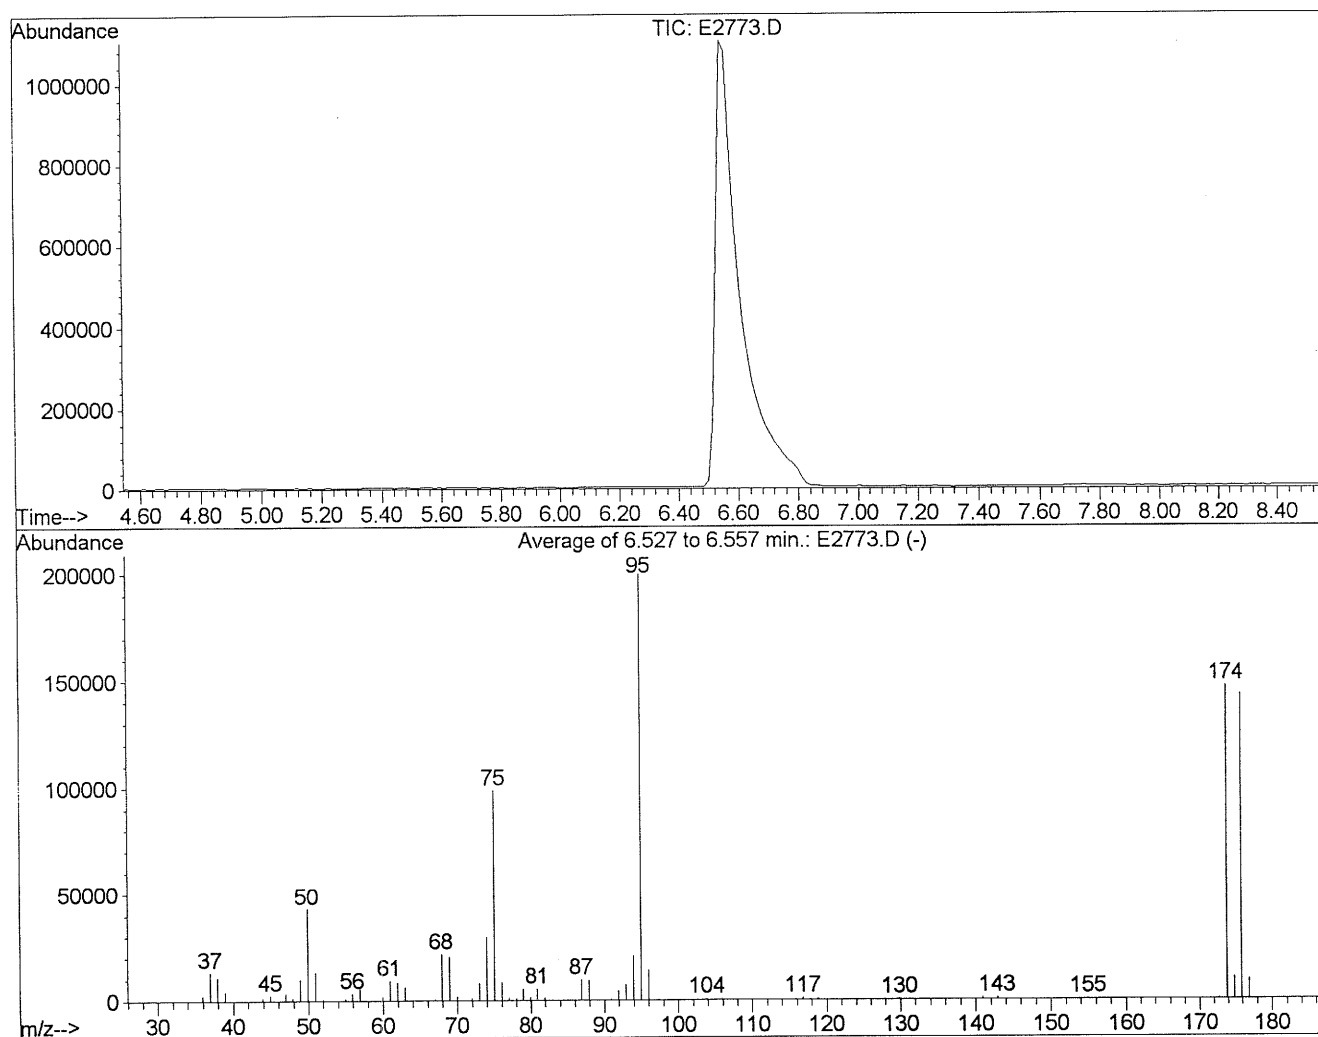


AutoFind: Scans 169, 170, 171; Background Corrected with Scan 164

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	43061	PASS
75	95	30	60	49.5	98760	PASS
95	95	100	100	100.0	199573	PASS
96	95	5	9	7.0	14052	PASS
173	174	0.00	2	0.2	246	PASS
174	95	50	100	73.7	147000	PASS
175	174	5	9	7.0	10327	PASS
176	174	95	101	97.4	143173	PASS
177	176	5	9	6.5	9341	PASS

C:\HPCHEM\1\DATA\042905\E2773.D

Fri Apr 29 08:46:09 2005

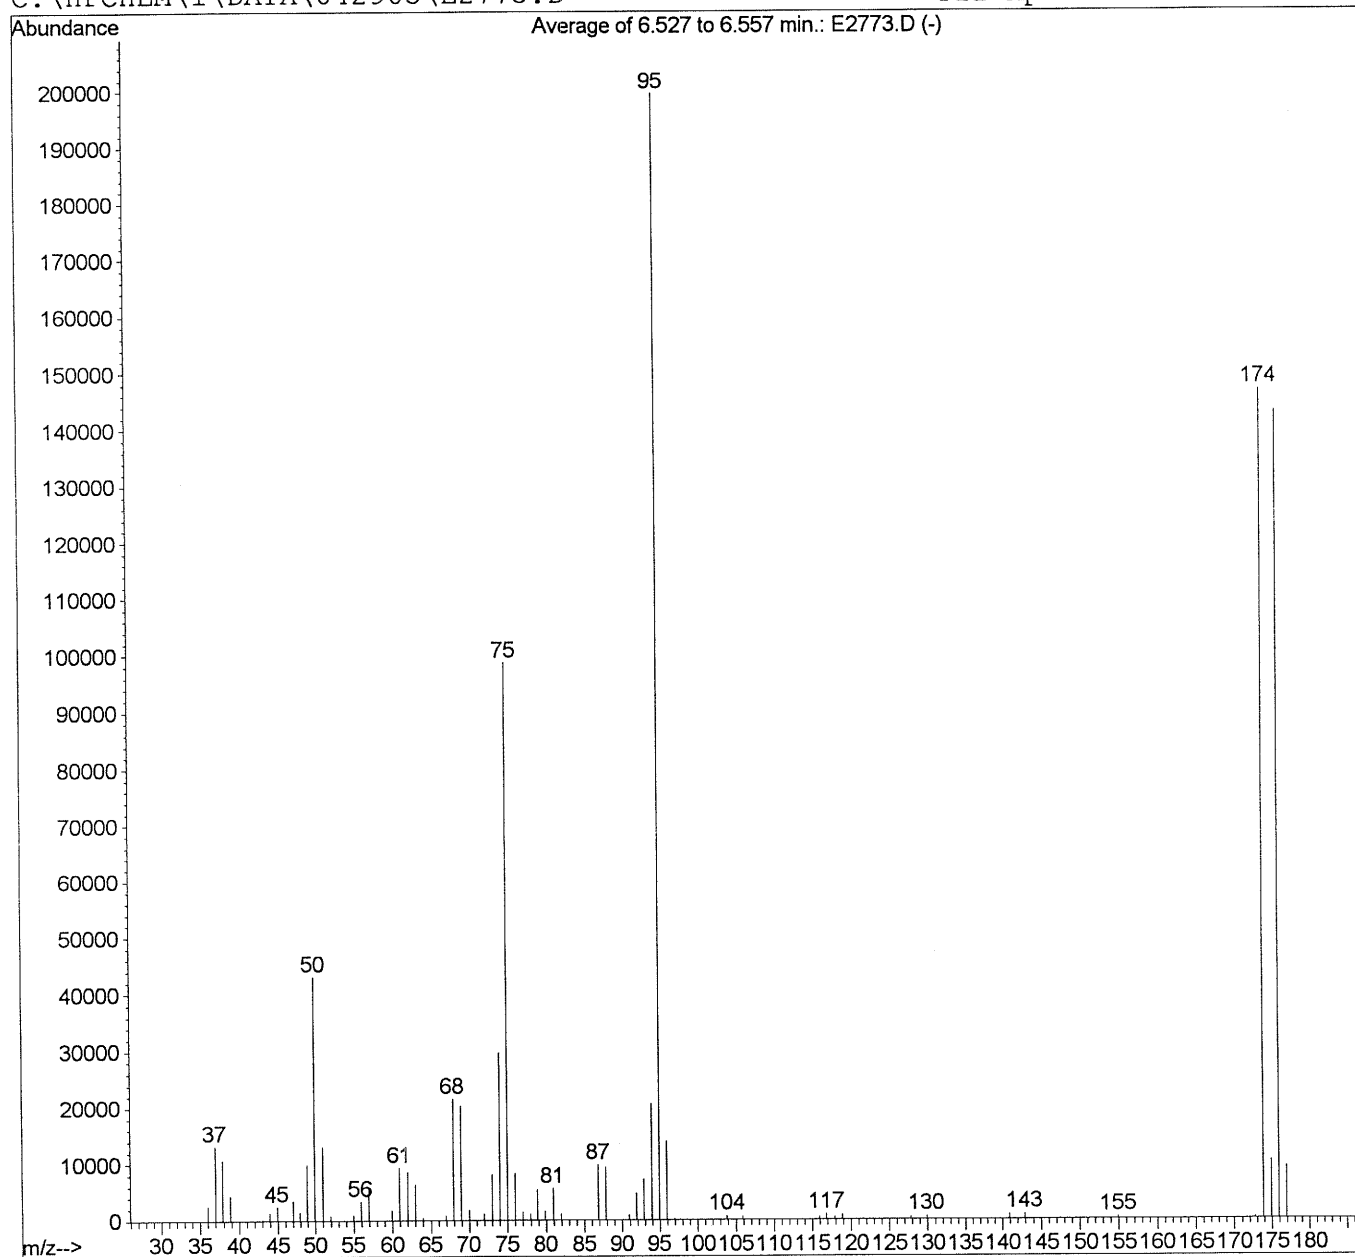

Peak Apex is scan: 170

Average of 3 scans: 169,170,171 minus background scan 164

Target	Comparison	Lower	Upper	Relative	Result
Mass	Mass	Limit,%	Limit,%	Abundance,%	Pass/Fail
50	95	15	40	21.6	PASS
75	95	30	60	49.5	PASS
95	95	100	100	100.0	PASS
96	95	5	9	7.0	PASS
173	174	0	2	0.2	PASS
174	95	50	100	73.7	PASS
175	174	5	9	7.0	PASS
176	174	95	101	97.4	PASS
177	176	5	9	6.5	PASS

RAW QC DATA

5A
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Toxikon Corporation Contract: _____
 Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209
 Lab File ID: C:\HPCHE BFB Injection Date: 4/1/2005
 Instrument ID: E BFB Injection Time: 7:37
 GC Column: RTX-624 ID: 0.32 (mm) Heated Purge: (Y/N) N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	8.0 - 40.0% of mass 95	22.1
75	30.0 - 66.0% of mass 95	50.3
95	Base peak, 100% relative abundance	100.0
96	5.0 - 9.0% of mass 95	7.1
173	Less than 2.0% of mass 174	0.0 (0.0)1
174	50.0 - 120.0% of mass 95	69.8
175	5.0 - 9.0% of mass 174	5.0 (7.1)1
176	95.0 - 101.0% of mass 174	68.7 (98.4)1
177	5.0 - 9.0% of mass 176	4.4 (6.4)2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS AND STANDARDS:

	EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
01	vstd005	vstd005	E2603.D	04/01/05	8:57
02	vstd010	vstd010	E2604.D	04/01/05	9:32
03	vstd020	vstd020	E2605.D	04/01/05	10:06
04	vstd050	vstd050	E2606.D	04/01/05	10:40
05	vstd100	vstd100	E2607.D	04/01/05	11:14
06	vstd200	vstd200	E2608.D	04/01/05	11:48

MBLK042905

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: MBLK042905

Sample wt/vol: _____ (g/mL) G Lab File ID: E2777.D

Level: (low/med) LOW Date Received: _____

% Moisture: not dec. Date Analyzed: 4/29/2005

GC Column: _____ ID: _____ (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CAS NO.	COMPOUND	CONCENTRATION UNITS:	
		(ug/L or ug/Kg)	µg/Kg Q
630-20-6	1,1,1,2-Tetrachloroethane	10	U
71-55-6	1,1,1-Trichloroethane	10	U
79-34-5	1,1,2,2-Tetrachloroethane	10	U
79-00-5	1,1,2-Trichloroethane	10	U
75-34-3	1,1-Dichloroethane	10	U
75-35-4	1,1-Dichloroethene	10	U
563-58-6	1,1-Dichloropropene	10	U
87-61-6	1,2,3-Trichlorobenzene	10	U
96-18-4	1,2,3-Trichloropropane	10	U
120-82-1	1,2,4-Trichlorobenzene	10	U
95-63-6	1,2,4-Trimethylbenzene	10	U
96-12-8	1,2-Dibromo-3-chloropropane	10	U
106-93-4	1,2-Dibromoethane	10	U
95-50-1	1,2-Dichlorobenzene	10	U
107-06-2	1,2-Dichloroethane	10	U
78-87-5	1,2-Dichloropropane	10	U
108-67-8	1,3,5-Trimethylbenzene	10	U
541-73-1	1,3-Dichlorobenzene	10	U
142-28-9	1,3-Dichloropropane	10	U
106-46-7	1,4-Dichlorobenzene	10	U
590-20-7	2,2-Dichloropropane	10	U
78-93-3	2-Butanone	10	U
110-75-8	2-Chloroethyl vinyl ether	10	U
95-49-8	2-Chlorotoluene	10	U
591-78-6	2-Hexanone	10	U
106-43-4	4-Chlorotoluene	10	U
99-87-6	4-Isopropyltoluene	10	U
108-10-1	4-Methyl-2-pentanone	10	U
67-64-1	Acetone	10	U
107-13-1	Acrylonitrile	100	U
71-43-2	Benzene	10	U
108-86-1	Bromobenzene	10	U
74-97-5	Bromochloromethane	10	U
75-27-4	Bromodichloromethane	10	U
75-25-2	Bromoform	10	U

MBLK042905

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: MBLK042905

Sample wt/vol: _____ (g/mL) G Lab File ID: E2777.D

Level: (low/med) LOW Date Received: _____

% Moisture: not dec. Date Analyzed: 4/29/2005

GC Column: _____ ID: _____ (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane		10	U
75-15-0	Carbon disulfide		10	U
56-23-5	Carbon tetrachloride		10	U
108-90-7	Chlorobenzene		10	U
75-00-3	Chloroethane		10	U
67-66-3	Chloroform		10	U
74-87-3	Chloromethane		10	U
156-59-2	cis-1,2-Dichloroethene		10	U
10061-01-5	cis-1,3-Dichloropropene		10	U
124-48-1	Dibromochloromethane		10	U
74-95-3	Dibromomethane		10	U
75-71-8	Dichlorodifluoromethane		10	U
100-41-4	Ethylbenzene		10	U
87-68-3	Hexachlorobutadiene		10	U
74-88-4	Iodomethane		10	U
98-82-8	Isopropylbenzene		10	U
1634-04-4	Methyl tert-butyl-ether		10	U
75-09-2	Methylene chloride		10	U
104-51-8	n-Butylbenzene		10	U
103-65-1	n-Propylbenzene		10	U
91-20-3	Naphthalene		10	U
135-98-8	sec-Butylbenzene		10	U
100-42-5	Styrene		10	U
98-06-6	tert-Butylbenzene		10	U
127-18-4	Tetrachloroethene		10	U
109-99-9	Tetrahydrofuran		10	U
108-88-3	Toluene		10	U
156-60-5	trans-1,2-Dichloroethene		10	U
10061-02-6	trans-1,3-Dichloropropene		10	U
79-01-6	Trichloroethene		10	U
75-69-4	Trichlorofluoromethane		10	U
108-05-4	Vinyl acetate		10	U
75-01-4	Vinyl chloride		10	U
1330-20-7	Xylenes, Total		10	U

MBLK042905

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: MBLK042905

Sample wt/vol: 5 (g/mL) G Lab File ID: E2777.D

Level: (low/med) LOW Date Received: _____

% Moisture: not dec. Date Analyzed: 4/29/2005

GC Column: RTX-624 ID: 0.32 (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CAS NO.	COMPOUND	CONCENTRATION UNITS:	
		(ug/L or ug/Kg)	µg/Kg Q
630-20-6	1,1,1,2-Tetrachloroethane	10	U
71-55-6	1,1,1-Trichloroethane	10	U
79-34-5	1,1,2,2-Tetrachloroethane	10	U
79-00-5	1,1,2-Trichloroethane	10	U
75-34-3	1,1-Dichloroethane	10	U
75-35-4	1,1-Dichloroethene	10	U
563-58-6	1,1-Dichloropropene	3.8	DJ
87-61-6	1,2,3-Trichlorobenzene	10	U
96-18-4	1,2,3-Trichloropropane	10	U
120-82-1	1,2,4-Trichlorobenzene	10	U
95-63-6	1,2,4-Trimethylbenzene	10	U
96-12-8	1,2-Dibromo-3-chloropropane	10	U
106-93-4	1,2-Dibromoethane	10	U
95-50-1	1,2-Dichlorobenzene	10	U
107-06-2	1,2-Dichloroethane	10	U
78-87-5	1,2-Dichloropropane	10	U
108-67-8	1,3,5-Trimethylbenzene	10	U
541-73-1	1,3-Dichlorobenzene	10	U
142-28-9	1,3-Dichloropropane	10	U
106-46-7	1,4-Dichlorobenzene	10	U
590-20-7	2,2-Dichloropropane	10	U
78-93-3	2-Butanone	10	U
110-75-8	2-Chloroethyl vinyl ether	10	U
95-49-8	2-Chlorotoluene	10	U
591-78-6	2-Hexanone	10	U
106-43-4	4-Chlorotoluene	10	U
99-87-6	4-Isopropyltoluene	10	U
108-10-1	4-Methyl-2-pentanone	10	U
67-64-1	Acetone	10	U
107-13-1	Acrylonitrile	100	U
71-43-2	Benzene	10	U
108-86-1	Bromobenzene	10	U
74-97-5	Bromochloromethane	10	U
75-27-4	Bromodichloromethane	10	U
75-25-2	Bromoform	10	U

MBLK042905

Lab Name: Toxikon Corporation Contract: _____
 Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209
 Matrix: (soil/water) Soil Lab Sample ID: MBLK042905
 Sample wt/vol: 5 (g/mL) G Lab File ID: E2777.D
 Level: (low/med) LOW Date Received: _____
 % Moisture: not dec. Date Analyzed: 4/29/2005
 GC Column: RTX-624 ID: 0.32 (mm) Dilution Factor: 1.00
 Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane	10	U	
75-15-0	Carbon disulfide	10	U	
56-23-5	Carbon tetrachloride	2.4	DJ	
108-90-7	Chlorobenzene	10	U	
75-00-3	Chloroethane	10	U	
67-66-3	Chloroform	10	U	
74-87-3	Chloromethane	10	U	
156-59-2	cis-1,2-Dichloroethene	10	U	
10061-01-5	cis-1,3-Dichloropropene	10	U	
124-48-1	Dibromochloromethane	10	U	
74-95-3	Dibromomethane	10	U	
75-71-8	Dichlorodifluoromethane	10	U	
100-41-4	Ethylbenzene	10	U	
87-68-3	Hexachlorobutadiene	10	U	
74-88-4	Iodomethane	10	U	
98-82-8	Isopropylbenzene	10	U	
1634-04-4	Methyl tert-butyl-ether	10	U	
75-09-2	Methylene chloride	10	U	
104-51-8	n-Butylbenzene	10	U	
103-65-1	n-Propylbenzene	10	U	
91-20-3	Naphthalene	10	U	
135-98-8	sec-Butylbenzene	10	U	
100-42-5	Styrene	10	U	
98-06-6	tert-Butylbenzene	10	U	
127-18-4	Tetrachloroethene	10	U	
109-99-9	Tetrahydrofuran	10	U	
108-88-3	Toluene	10	U	
156-60-5	trans-1,2-Dichloroethene	10	U	
10061-02-6	trans-1,3-Dichloropropene	10	U	
79-01-6	Trichloroethene	3.2	DJ	
75-69-4	Trichlorofluoromethane	10	U	
108-05-4	Vinyl acetate	10	U	
75-01-4	Vinyl chloride	10	U	
1330-20-7	Xylenes, Total	10	U	

Data File : C:\HPCHEM\1\DATA\042905\E2777.D
Acq On : 29 Apr 05 10:51 am
Sample : MBLK042905
Misc : MBLK asp_8260s
MS Integration Params: rteint.p
Quant Time: May 2 6:01 19105

Vial: 4
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Mon Apr 04 10:16:13 2005
Response via : Initial Calibration
DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.61	168	1836227	50.00	ug/Kg	0.00
32) 1,4-difluorobenzene	8.80	114	3266877	50.00	ug/Kg	0.02
49) chlorobenzene-d5	13.95	117	3139439	50.00	ug/Kg	0.02
63) 1,4-dichlorobenzene-d4	18.44	152	1426490	50.00	ug/Kg	0.02

System Monitoring Compounds

29) Dibromofluoromethane	7.49	113	1084954	47.34	ug/Kg	0.02
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.68%
45) toluene-d8	11.28	98	3744884	49.00	ug/Kg	0.02
Spiked Amount	50.000	Range	81 - 120	Recovery	=	98.00%
62) 4-Bromofluorobenzene	16.22	95	1477286	48.80	ug/Kg	0.02
Spiked Amount	50.000	Range	74 - 121	Recovery	=	97.60%

Target Compounds

10) Acetone	3.79	43	18809	1.10 ug/Kg	Qvalue	95
-------------	------	----	-------	-----------------------	--------	----

(#) = qualifier out of range (m) = manual integration

E2777.D 8260ES6.M Mon May 02 06:01:15 2005

Page 1

000148


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2777.D
 Acq On : 29 Apr 05 10:51 am
 Sample : MBLK042905
 Misc : MBLK asp_8260s
 MS Integration Params: rteint.p
 Quant Time: May 2 6:01 19105

Vial: 4
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

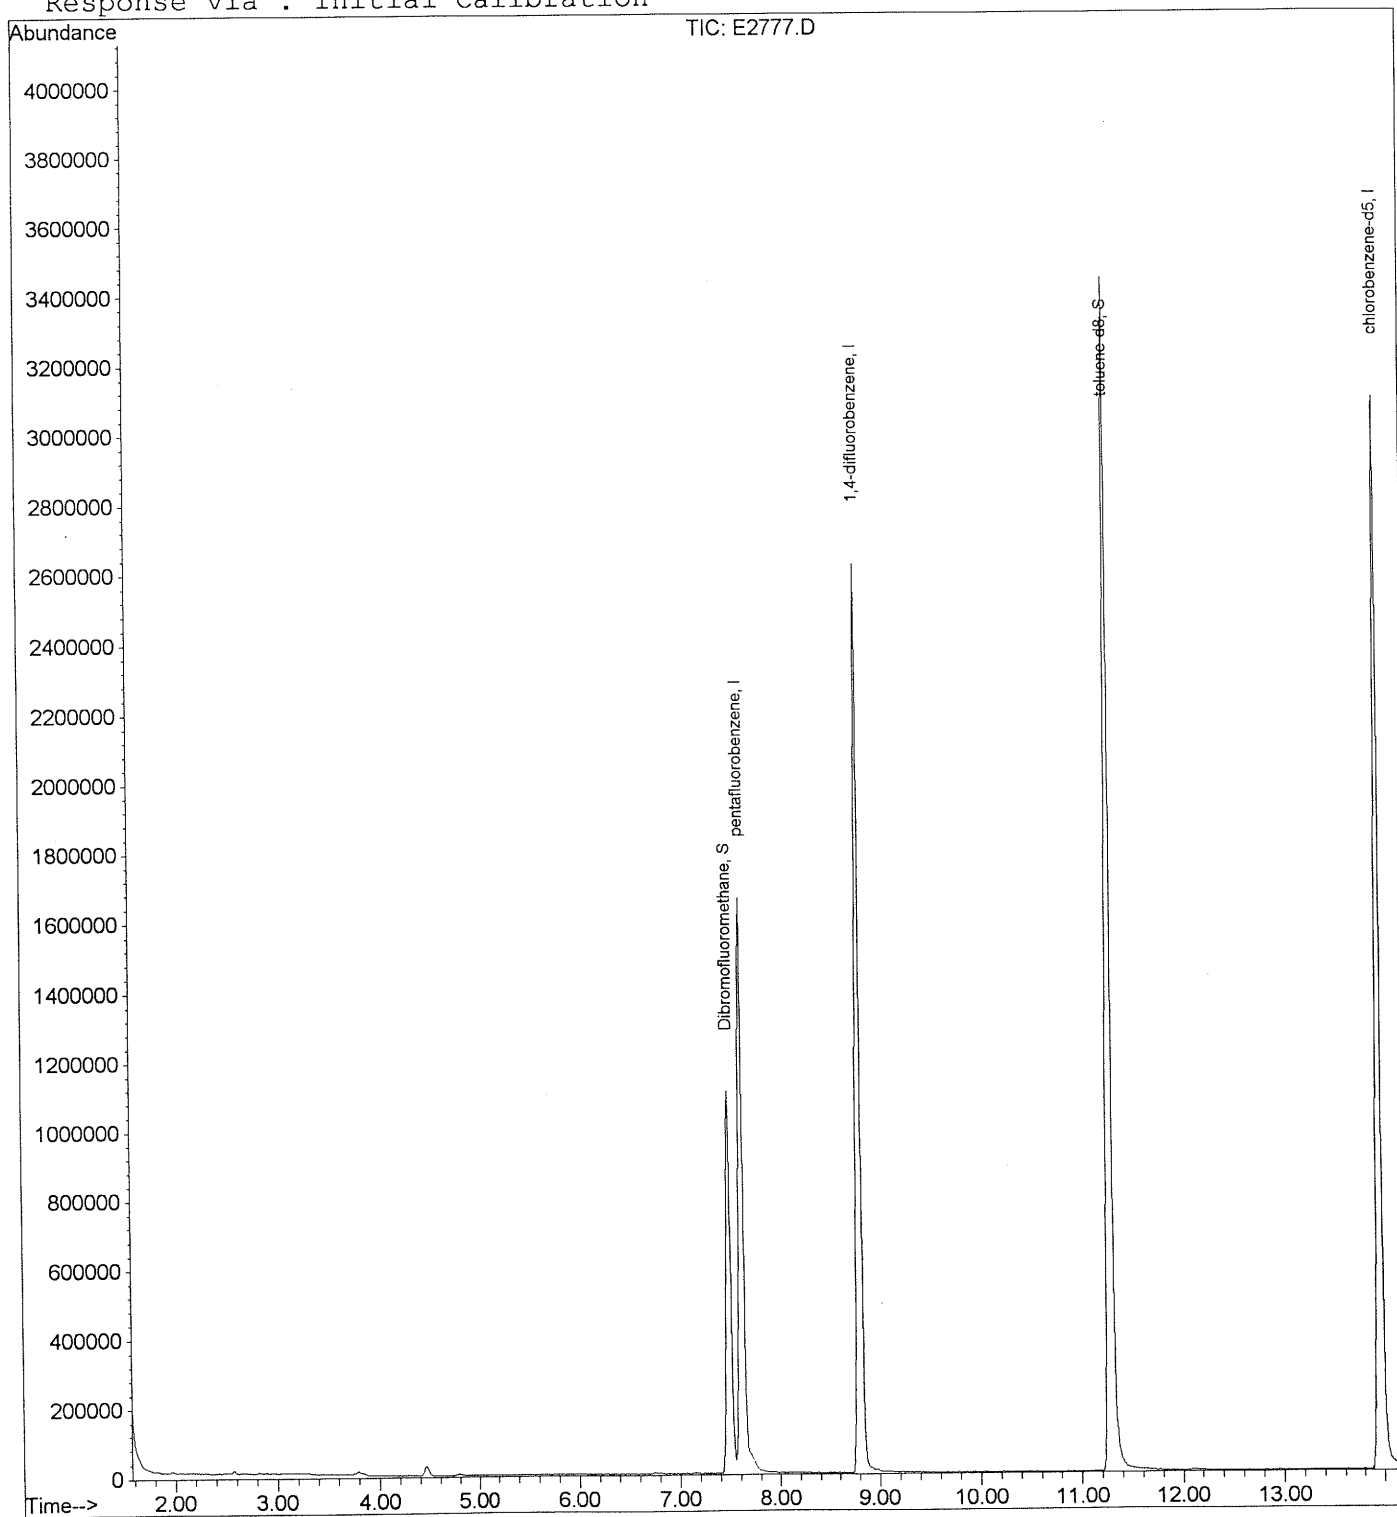


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2777.D
 Acq On : 29 Apr 05 10:51 am
 Sample : MBLK042905
 Misc : MBLK asp_8260s
 MS Integration Params: rteint.p
 Quant Time: May 2 6:01 19105

Vial: 4
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

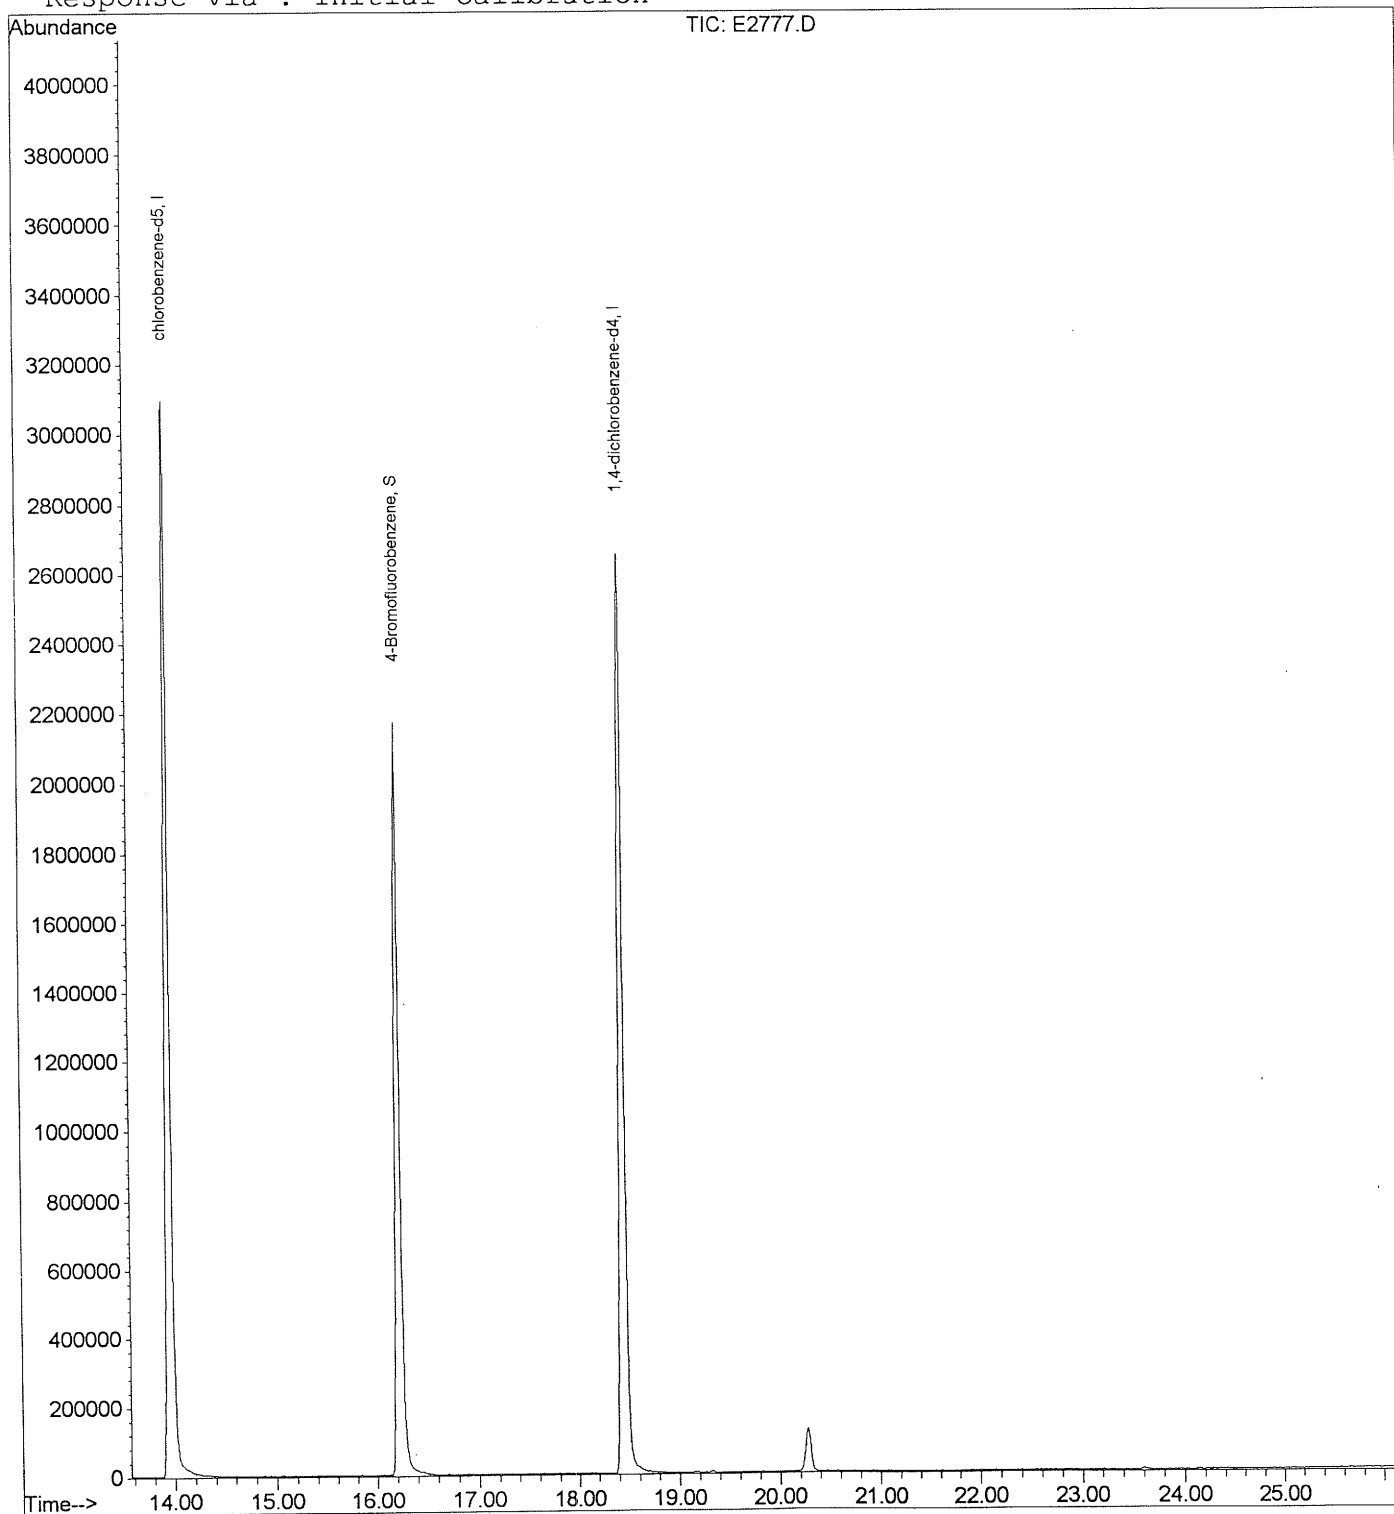

Lab Name: Toxikon Corporation

Contract: _____

MW-2 B (43-45)MS

Lab Code: 10778Case No.: LBG WHIT SAS No.: _____SDG No.: 0504209

Matrix: (soil/water)

SoilLab Sample ID: 0504209-04A

Sample wt/vol:

5 (g/mL) GLab File ID: E2785.D

Level: (low/med)

LOWDate Received: 4/27/2005

% Moisture: not dec.

12.7Date Analyzed: 4/29/2005GC Column: RTX-624ID: 0.32 (mm)Dilution Factor: 1.00

Extract Volume: _____

(µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
630-20-6	1,1,1,2-Tetrachloroethane	12		U
71-55-6	1,1,1-Trichloroethane	12		U
79-34-5	1,1,2,2-Tetrachloroethane	12		U
79-00-5	1,1,2-Trichloroethane	12		U
75-34-3	1,1-Dichloroethane	12		U
75-35-4	1,1-Dichloroethene	58.1		D
563-58-6	1,1-Dichloropropene	12		U
87-61-6	1,2,3-Trichlorobenzene	12		U
96-18-4	1,2,3-Trichloropropane	12		U
120-82-1	1,2,4-Trichlorobenzene	12		U
95-63-6	1,2,4-Trimethylbenzene	12		U
96-12-8	1,2-Dibromo-3-chloropropane	12		U
106-93-4	1,2-Dibromoethane	12		U
95-50-1	1,2-Dichlorobenzene	12		U
107-06-2	1,2-Dichloroethane	12		U
78-87-5	1,2-Dichloropropane	12		U
108-67-8	1,3,5-Trimethylbenzene	12		U
541-73-1	1,3-Dichlorobenzene	12		U
142-28-9	1,3-Dichloropropane	12		U
106-46-7	1,4-Dichlorobenzene	12		U
590-20-7	2,2-Dichloropropane	12		U
78-93-3	2-Butanone	12		U
110-75-8	2-Chloroethyl vinyl ether	428		DE
95-49-8	2-Chlorotoluene	12		U
591-78-6	2-Hexanone	12		U
106-43-4	4-Chlorotoluene	12		U
99-87-6	4-Isopropyltoluene	12		U
108-10-1	4-Methyl-2-pentanone	12		U
67-64-1	Acetone	12		U
107-13-1	Acrylonitrile	120		U
71-43-2	Benzene	57.2		D
108-86-1	Bromobenzene	12		U
74-97-5	Bromochloromethane	12		U
75-27-4	Bromodichloromethane	12		U
75-25-2	Bromoform	12		U

MW-2 B (43-45)MS

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 0504209-04A

Sample wt/vol: 5 (g/mL) G Lab File ID: E2785.D

Level: (low/med) LOW Date Received: 4/27/2005

% Moisture: not dec. 12.7 Date Analyzed: 4/29/2005

GC Column: RTX-624 ID: 0.32 (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane	12		U
75-15-0	Carbon disulfide	12		U
56-23-5	Carbon tetrachloride	2.5		DBJ
108-90-7	Chlorobenzene	58.0		D
75-00-3	Chloroethane	12		U
67-66-3	Chloroform	12		U
74-87-3	Chloromethane	12		U
156-59-2	cis-1,2-Dichloroethene	12		U
10061-01-5	cis-1,3-Dichloropropene	12		U
124-48-1	Dibromochloromethane	12		U
74-95-3	Dibromomethane	12		U
75-71-8	Dichlorodifluoromethane	12		U
100-41-4	Ethylbenzene	12		U
87-68-3	Hexachlorobutadiene	12		U
74-88-4	Iodomethane	12		U
98-82-8	Isopropylbenzene	12		U
1634-04-4	Methyl tert-butyl-ether	12		U
75-09-2	Methylene chloride	12		U
104-51-8	n-Butylbenzene	12		U
103-65-1	n-Propylbenzene	12		U
91-20-3	Naphthalene	12		U
135-98-8	sec-Butylbenzene	12		U
100-42-5	Styrene	12		U
98-06-6	tert-Butylbenzene	12		U
127-18-4	Tetrachloroethene	7.5		DJ
109-99-9	Tetrahydrofuran	12		U
108-88-3	Toluene	58.1		D
156-60-5	trans-1,2-Dichloroethene	12		U
10061-02-6	trans-1,3-Dichloropropene	12		U
79-01-6	Trichloroethene	56.6		DB
75-69-4	Trichlorofluoromethane	12		U
108-05-4	Vinyl acetate	12		U
75-01-4	Vinyl chloride	12		U
1330-20-7	Xylenes, Total	12		U

MW-2 B (43-45)MS

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 0504209-04A

Sample wt/vol: _____ (g/mL) G Lab File ID: E2785.D

Level: (low/med) LOW Date Received: 4/27/2005

% Moisture: not dec. 12.7 Date Analyzed: 4/29/2005

GC Column: _____ ID: _____ (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
630-20-6	1,1,1,2-Tetrachloroethane	12		U
71-55-6	1,1,1-Trichloroethane	12		U
79-34-5	1,1,2,2-Tetrachloroethane	12		U
79-00-5	1,1,2-Trichloroethane	12		U
75-34-3	1,1-Dichloroethane	12		U
75-35-4	1,1-Dichloroethene	58.1		D
563-58-6	1,1-Dichloropropene	12		U
87-61-6	1,2,3-Trichlorobenzene	12		U
96-18-4	1,2,3-Trichloropropane	12		U
120-82-1	1,2,4-Trichlorobenzene	12		U
95-63-6	1,2,4-Trimethylbenzene	12		U
96-12-8	1,2-Dibromo-3-chloropropane	12		U
106-93-4	1,2-Dibromoethane	12		U
95-50-1	1,2-Dichlorobenzene	12		U
107-06-2	1,2-Dichloroethane	12		U
78-87-5	1,2-Dichloropropane	12		U
108-67-8	1,3,5-Trimethylbenzene	12		U
541-73-1	1,3-Dichlorobenzene	12		U
142-28-9	1,3-Dichloropropane	12		U
106-46-7	1,4-Dichlorobenzene	12		U
590-20-7	2,2-Dichloropropane	12		U
78-93-3	2-Butanone	12		U
110-75-8	2-Chloroethyl vinyl ether	12		U
95-49-8	2-Chlorotoluene	12		U
591-78-6	2-Hexanone	12		U
106-43-4	4-Chlorotoluene	12		U
99-87-6	4-Isopropyltoluene	12		U
108-10-1	4-Methyl-2-pentanone	12		U
67-64-1	Acetone	12		U
107-13-1	Acrylonitrile	120		U
71-43-2	Benzene	57.2		D
108-86-1	Bromobenzene	12		U
74-97-5	Bromochloromethane	12		U
75-27-4	Bromodichloromethane	12		U
75-25-2	Bromoform	12		U

MW-2 B (43-45)MS

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 0504209-04A

Sample wt/vol: _____ (g/mL) G Lab File ID: E2785.D

Level: (low/med) LOW Date Received: 4/27/2005

% Moisture: not dec. 12.7 Date Analyzed: 4/29/2005

GC Column: _____ ID: _____ (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane	12		U
75-15-0	Carbon disulfide	12		U
56-23-5	Carbon tetrachloride	12		U
108-90-7	Chlorobenzene	58.0		D
75-00-3	Chloroethane	12		U
67-66-3	Chloroform	12		U
74-87-3	Chloromethane	12		U
156-59-2	cis-1,2-Dichloroethene	12		U
10061-01-5	cis-1,3-Dichloropropene	12		U
124-48-1	Dibromochloromethane	12		U
74-95-3	Dibromomethane	12		U
75-71-8	Dichlorodifluoromethane	12		U
100-41-4	Ethylbenzene	12		U
87-68-3	Hexachlorobutadiene	12		U
74-88-4	Iodomethane	12		U
98-82-8	Isopropylbenzene	12		U
1634-04-4	Methyl tert-butyl-ether	12		U
75-09-2	Methylene chloride	12		U
104-51-8	n-Butylbenzene	12		U
103-65-1	n-Propylbenzene	12		U
91-20-3	Naphthalene	12		U
135-98-8	sec-Butylbenzene	12		U
100-42-5	Styrene	12		U
98-06-6	tert-Butylbenzene	12		U
127-18-4	Tetrachloroethene	7.5		DJ
109-99-9	Tetrahydrofuran	12		U
108-88-3	Toluene	58.1		D
156-60-5	trans-1,2-Dichloroethene	12		U
10061-02-6	trans-1,3-Dichloropropene	12		U
79-01-6	Trichloroethene	56.6		D
75-69-4	Trichlorofluoromethane	12		U
108-05-4	Vinyl acetate	12		U
75-01-4	Vinyl chloride	12		U
1330-20-7	Xylenes, Total	12		U

Data File : C:\HPCHEM\1\DATA\042905\E2785.D

Vial: 12

Acq On : 29 Apr 05 3:31 pm

Operator: xl

Sample : 0504209-04ams

Inst : inst e

Misc : ms asp_8260s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: May 2 6:19 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Apr 04 10:16:13 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.61	168	1832148	50.00	ug/Kg	0.00
32) 1,4-difluorobenzene	8.80	114	3358373	50.00	ug/Kg	0.02
49) chlorobenzene-d5	13.95	117	3222165	50.00	ug/Kg	0.02
63) 1,4-dichlorobenzene-d4	18.44	152	1445976	50.00	ug/Kg	0.02

System Monitoring Compounds

29) Dibromofluoromethane	7.49	113	1100809	48.13	ug/Kg	0.02
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.26%
45) toluene-d8	11.28	98	3840365	48.88	ug/Kg	0.02
Spiked Amount	50.000	Range	81 - 120	Recovery	=	97.76%
62) 4-Bromofluorobenzene	16.21	95	1513878	48.73	ug/Kg	0.02
Spiked Amount	50.000	Range	74 - 121	Recovery	=	97.46%

Target Compounds

					Qvalue	
12) 1,1-dichloroethene	3.56	96	764460	50.70	ug/Kg	95
35) benzene	8.00	78	4970261	49.91	ug/Kg	100
38) trichloroethene	9.16	95	1369026	49.41	ug/Kg	100
46) toluene	11.40	92	3149756	50.74	ug/Kg	99
51) tetrachloroethene	12.33	166	162797	6.53	ug/Kg	99
55) chlorobenzene	14.00	112	3503299	50.60	ug/Kg	99

XL 5/2/05


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2785.D
Acq On : 29 Apr 05 3:31 pm
Sample : 0504209-04ams
Misc : ms asp_8260s
MS Integration Params: rteint.p
Quant Time: May 2 6:19 19105

Vial: 12
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Mon Apr 04 10:16:13 2005
Response via : Initial Calibration

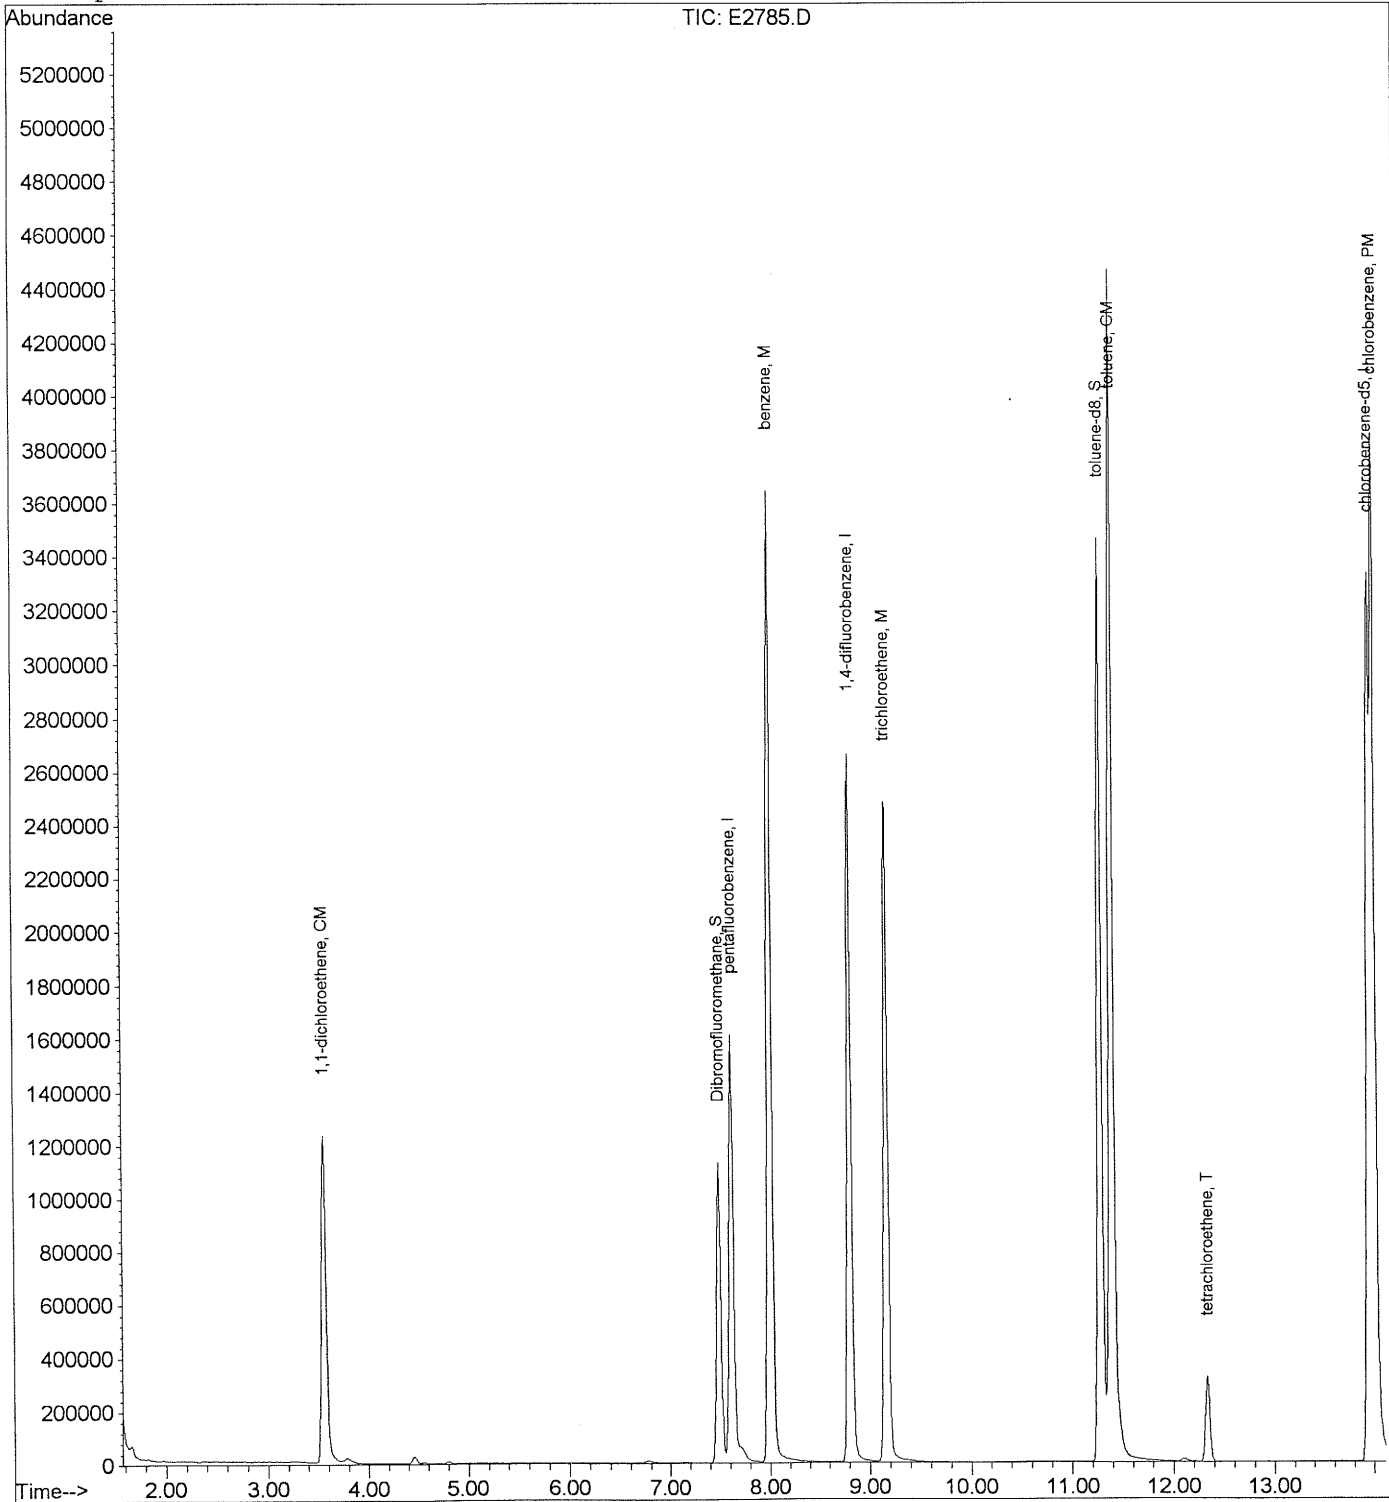


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2785.D
Acq On : 29 Apr 05 3:31 pm
Sample : 0504209-04ams
Misc : ms asp_8260s
MS Integration Params: rteint.p
Quant Time: May 2 6:19 19105

Vial: 12
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Mon Apr 04 10:16:13 2005
Response via : Initial Calibration

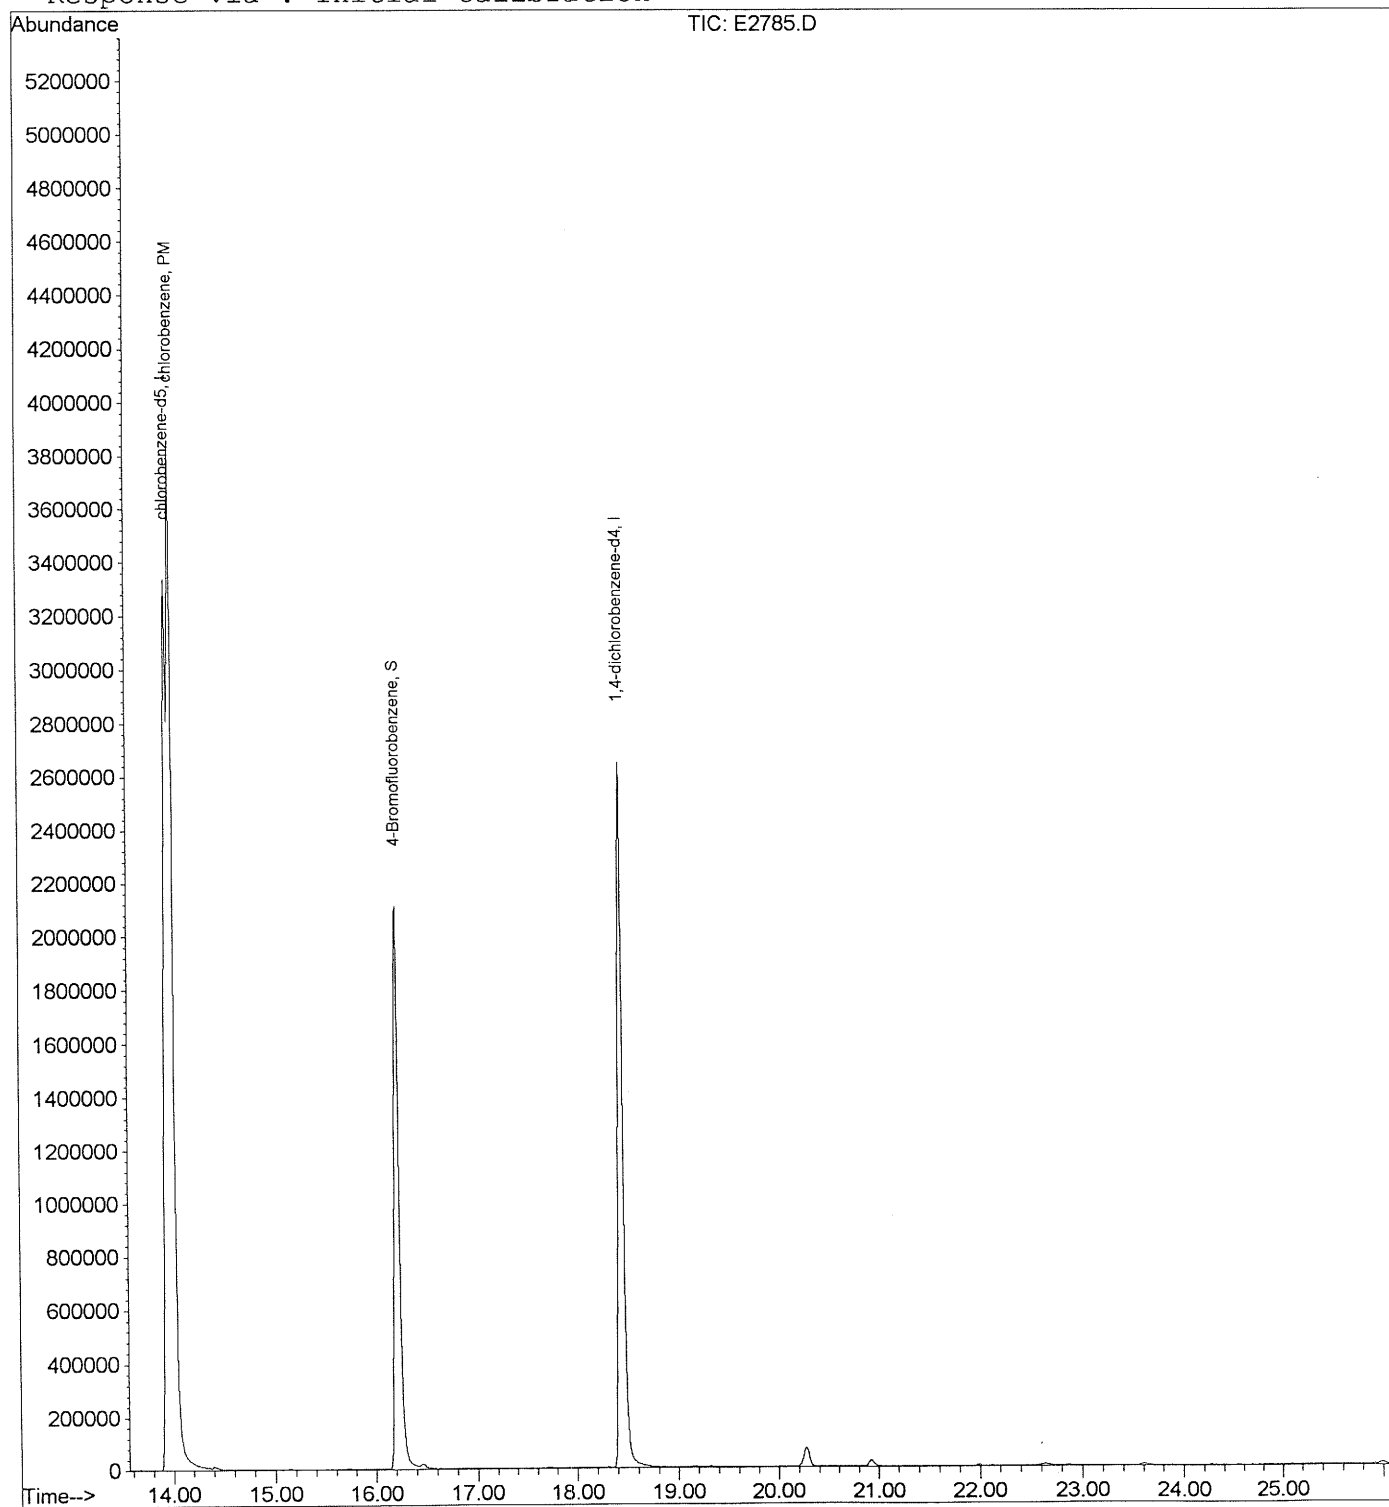

MW-2 B (43-45)MSD

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 0504209-04A

Sample wt/vol: _____ (g/mL) G Lab File ID: E2786.D

Level: (low/med) LOW Date Received: 4/27/2005

% Moisture: not dec. 12.7 Date Analyzed: 4/29/2005

GC Column: _____ ID: _____ (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
630-20-6	1,1,1,2-Tetrachloroethane	12		U
71-55-6	1,1,1-Trichloroethane	12		U
79-34-5	1,1,2,2-Tetrachloroethane	12		U
79-00-5	1,1,2-Trichloroethane	12		U
75-34-3	1,1-Dichloroethane	12		U
75-35-4	1,1-Dichloroethene	56.7		D
563-58-6	1,1-Dichloropropene	12		U
87-61-6	1,2,3-Trichlorobenzene	12		U
96-18-4	1,2,3-Trichloropropane	12		U
120-82-1	1,2,4-Trichlorobenzene	12		U
95-63-6	1,2,4-Trimethylbenzene	12		U
96-12-8	1,2-Dibromo-3-chloropropane	12		U
106-93-4	1,2-Dibromoethane	12		U
95-50-1	1,2-Dichlorobenzene	12		U
107-06-2	1,2-Dichloroethane	12		U
78-87-5	1,2-Dichloropropane	12		U
108-67-8	1,3,5-Trimethylbenzene	12		U
541-73-1	1,3-Dichlorobenzene	12		U
142-28-9	1,3-Dichloropropane	12		U
106-46-7	1,4-Dichlorobenzene	12		U
590-20-7	2,2-Dichloropropane	12		U
78-93-3	2-Butanone	12		U
110-75-8	2-Chloroethyl vinyl ether	12		U
95-49-8	2-Chlorotoluene	12		U
591-78-6	2-Hexanone	12		U
106-43-4	4-Chlorotoluene	12		U
99-87-6	4-Isopropyltoluene	12		U
108-10-1	4-Methyl-2-pentanone	12		U
67-64-1	Acetone	12		U
107-13-1	Acrylonitrile	120		U
71-43-2	Benzene	57.4		D
108-86-1	Bromobenzene	12		U
74-97-5	Bromochloromethane	12		U
75-27-4	Bromodichloromethane	12		U
75-25-2	Bromoform	12		U

Lab Name: Toxikon Corporation

Contract: _____

MW-2 B (43-45)MSD

Lab Code: 10778Case No.: LBG WHIT SAS No.: _____SDG No.: 0504209

Matrix: (soil/water)

SoilLab Sample ID: 0504209-04A

Sample wt/vol:

(g/mL) GLab File ID: E2786.D

Level: (low/med)

LOWDate Received: 4/27/2005

% Moisture: not dec.

12.7Date Analyzed: 4/29/2005

GC Column:

ID: (mm)

Dilution Factor: 1.00

Extract Volume: _____

(µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane	12		U
75-15-0	Carbon disulfide	12		U
56-23-5	Carbon tetrachloride	12		U
108-90-7	Chlorobenzene	55.4		D
75-00-3	Chloroethane	12		U
67-66-3	Chloroform	12		U
74-87-3	Chloromethane	12		U
156-59-2	cis-1,2-Dichloroethene	12		U
10061-01-5	cis-1,3-Dichloropropene	12		U
124-48-1	Dibromochloromethane	12		U
74-95-3	Dibromomethane	12		U
75-71-8	Dichlorodifluoromethane	12		U
100-41-4	Ethylbenzene	12		U
87-68-3	Hexachlorobutadiene	12		U
74-88-4	Iodomethane	12		U
98-82-8	Isopropylbenzene	12		U
1634-04-4	Methyl tert-butyl-ether	12		U
75-09-2	Methylene chloride	12		U
104-51-8	n-Butylbenzene	12		U
103-65-1	n-Propylbenzene	12		U
91-20-3	Naphthalene	12		U
135-98-8	sec-Butylbenzene	12		U
100-42-5	Styrene	12		U
98-06-6	tert-Butylbenzene	12		U
127-18-4	Tetrachloroethene	14.7		D
109-99-9	Tetrahydrofuran	12		U
108-88-3	Toluene	56.8		D
156-60-5	trans-1,2-Dichloroethene	12		U
10061-02-6	trans-1,3-Dichloropropene	12		U
79-01-6	Trichloroethene	54.6		D
75-69-4	Trichlorofluoromethane	12		U
108-05-4	Vinyl acetate	12		U
75-01-4	Vinyl chloride	12		U
1330-20-7	Xylenes, Total	12		U

Lab Name: Toxikon Corporation

Contract: _____

MW-2 B (43-45)MSD

Lab Code: 10778Case No.: LBG WHIT SAS No.: _____SDG No.: 0504209Matrix: (soil/water) SoilLab Sample ID: 0504209-04ASample wt/vol: 5 (g/mL) GLab File ID: E2786.DLevel: (low/med) LOWDate Received: 4/27/2005% Moisture: not dec. 12.7Date Analyzed: 4/29/2005GC Column: RTX-624 ID: 0.32 (mm)Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
630-20-6	1,1,1,2-Tetrachloroethane	12		U
71-55-6	1,1,1-Trichloroethane	12		U
79-34-5	1,1,2,2-Tetrachloroethane	12		U
79-00-5	1,1,2-Trichloroethane	12		U
75-34-3	1,1-Dichloroethane	12		U
75-35-4	1,1-Dichloroethene	56.7		D
563-58-6	1,1-Dichloropropene	4.4		DBJ
87-61-6	1,2,3-Trichlorobenzene	12		U
96-18-4	1,2,3-Trichloropropane	12		U
120-82-1	1,2,4-Trichlorobenzene	12		U
95-63-6	1,2,4-Trimethylbenzene	12		U
96-12-8	1,2-Dibromo-3-chloropropane	12		U
106-93-4	1,2-Dibromoethane	12		U
95-50-1	1,2-Dichlorobenzene	12		U
107-06-2	1,2-Dichloroethane	12		U
78-87-5	1,2-Dichloropropane	12		U
108-67-8	1,3,5-Trimethylbenzene	12		U
541-73-1	1,3-Dichlorobenzene	12		U
142-28-9	1,3-Dichloropropane	12		U
106-46-7	1,4-Dichlorobenzene	12		U
590-20-7	2,2-Dichloropropane	12		U
78-93-3	2-Butanone	12		U
110-75-8	2-Chloroethyl vinyl ether	424		DE
95-49-8	2-Chlorotoluene	12		U
591-78-6	2-Hexanone	12		U
106-43-4	4-Chlorotoluene	12		U
99-87-6	4-Isopropyltoluene	12		U
108-10-1	4-Methyl-2-pentanone	12		U
67-64-1	Acetone	12		U
107-13-1	Acrylonitrile	120		U
71-43-2	Benzene	57.4		D
108-86-1	Bromobenzene	12		U
74-97-5	Bromochloromethane	12		U
75-27-4	Bromodichloromethane	12		U
75-25-2	Bromoform	12		U

MW-2 B (43-45)MSD

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 0504209-04A

Sample wt/vol: 5 (g/mL) G Lab File ID: E2786.D

Level: (low/med) LOW Date Received: 4/27/2005

% Moisture: not dec. 12.7 Date Analyzed: 4/29/2005

GC Column: RTX-624 ID: 0.32 (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane	12	U	
75-15-0	Carbon disulfide	12	U	
56-23-5	Carbon tetrachloride	2.6	DBJ	
108-90-7	Chlorobenzene	55.4	D	
75-00-3	Chloroethane	12	U	
67-66-3	Chloroform	12	U	
74-87-3	Chloromethane	12	U	
156-59-2	cis-1,2-Dichloroethene	12	U	
10061-01-5	cis-1,3-Dichloropropene	12	U	
124-48-1	Dibromochloromethane	12	U	
74-95-3	Dibromomethane	12	U	
75-71-8	Dichlorodifluoromethane	12	U	
100-41-4	Ethylbenzene	12	U	
87-68-3	Hexachlorobutadiene	12	U	
74-88-4	Iodomethane	12	U	
98-82-8	Isopropylbenzene	12	U	
1634-04-4	Methyl tert-butyl-ether	12	U	
75-09-2	Methylene chloride	12	U	
104-51-8	n-Butylbenzene	12	U	
103-65-1	n-Propylbenzene	12	U	
91-20-3	Naphthalene	12	U	
135-98-8	sec-Butylbenzene	12	U	
100-42-5	Styrene	12	U	
98-06-6	tert-Butylbenzene	12	U	
127-18-4	Tetrachloroethene	14.7	D	
109-99-9	Tetrahydrofuran	12	U	
108-88-3	Toluene	56.8	D	
156-60-5	trans-1,2-Dichloroethene	12	U	
10061-02-6	trans-1,3-Dichloropropene	12	U	
79-01-6	Trichloroethene	54.6	DB	
75-69-4	Trichlorofluoromethane	12	U	
108-05-4	Vinyl acetate	12	U	
75-01-4	Vinyl chloride	12	U	
1330-20-7	Xylenes, Total	12	U	

Data File : C:\HPCHEM\1\DATA\042905\E2786.D
Acq On : 29 Apr 05 4:04 pm
Sample : 0504209-04amsd
Misc : msd asp_8260s
MS Integration Params: rteint.p
Quant Time: May 2 6:35 19105

Vial: 13
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Mon Apr 04 10:16:13 2005
Response via : Initial Calibration
DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.61	168	1822954	50.00	ug/Kg	0.00
32) 1,4-difluorobenzene	8.80	114	3312986	50.00	ug/Kg	0.02
49) chlorobenzene-d5	13.95	117	3235267	50.00	ug/Kg	0.02
63) 1,4-dichlorobenzene-d4	18.44	152	1448081	50.00	ug/Kg	0.02

System Monitoring Compounds

29) Dibromofluoromethane	7.49	113	1085241	47.69	ug/Kg	0.02
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.38%
45) toluene-d8	11.28	98	3817827	49.26	ug/Kg	0.02
Spiked Amount	50.000	Range	81 - 120	Recovery	=	98.52%
62) 4-Bromofluorobenzene	16.21	95	1508231	48.35	ug/Kg	0.02
Spiked Amount	50.000	Range	74 - 121	Recovery	=	96.70%

Target Compounds

					Qvalue
12) 1,1-dichloroethene	3.56	96	742980	49.52	ug/Kg 92
35) benzene	8.00	78	4920639	50.09	ug/Kg 100
38) trichloroethene	9.16	95	1303345	47.69	ug/Kg 98
46) toluene	11.40	92	3036021	49.58	ug/Kg 100
51) tetrachloroethene	12.33	166	321182	12.83	ug/Kg 97
55) chlorobenzene	14.00	112	3362936	48.38	ug/Kg 98

xl 5/105


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2786.D
 Acq On : 29 Apr 05 4:04 pm
 Sample : 0504209-04amsd
 Misc : msd asp_8260s
 MS Integration Params: rteint.p
 Quant Time: May 2 6:35 19105

Vial: 13
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

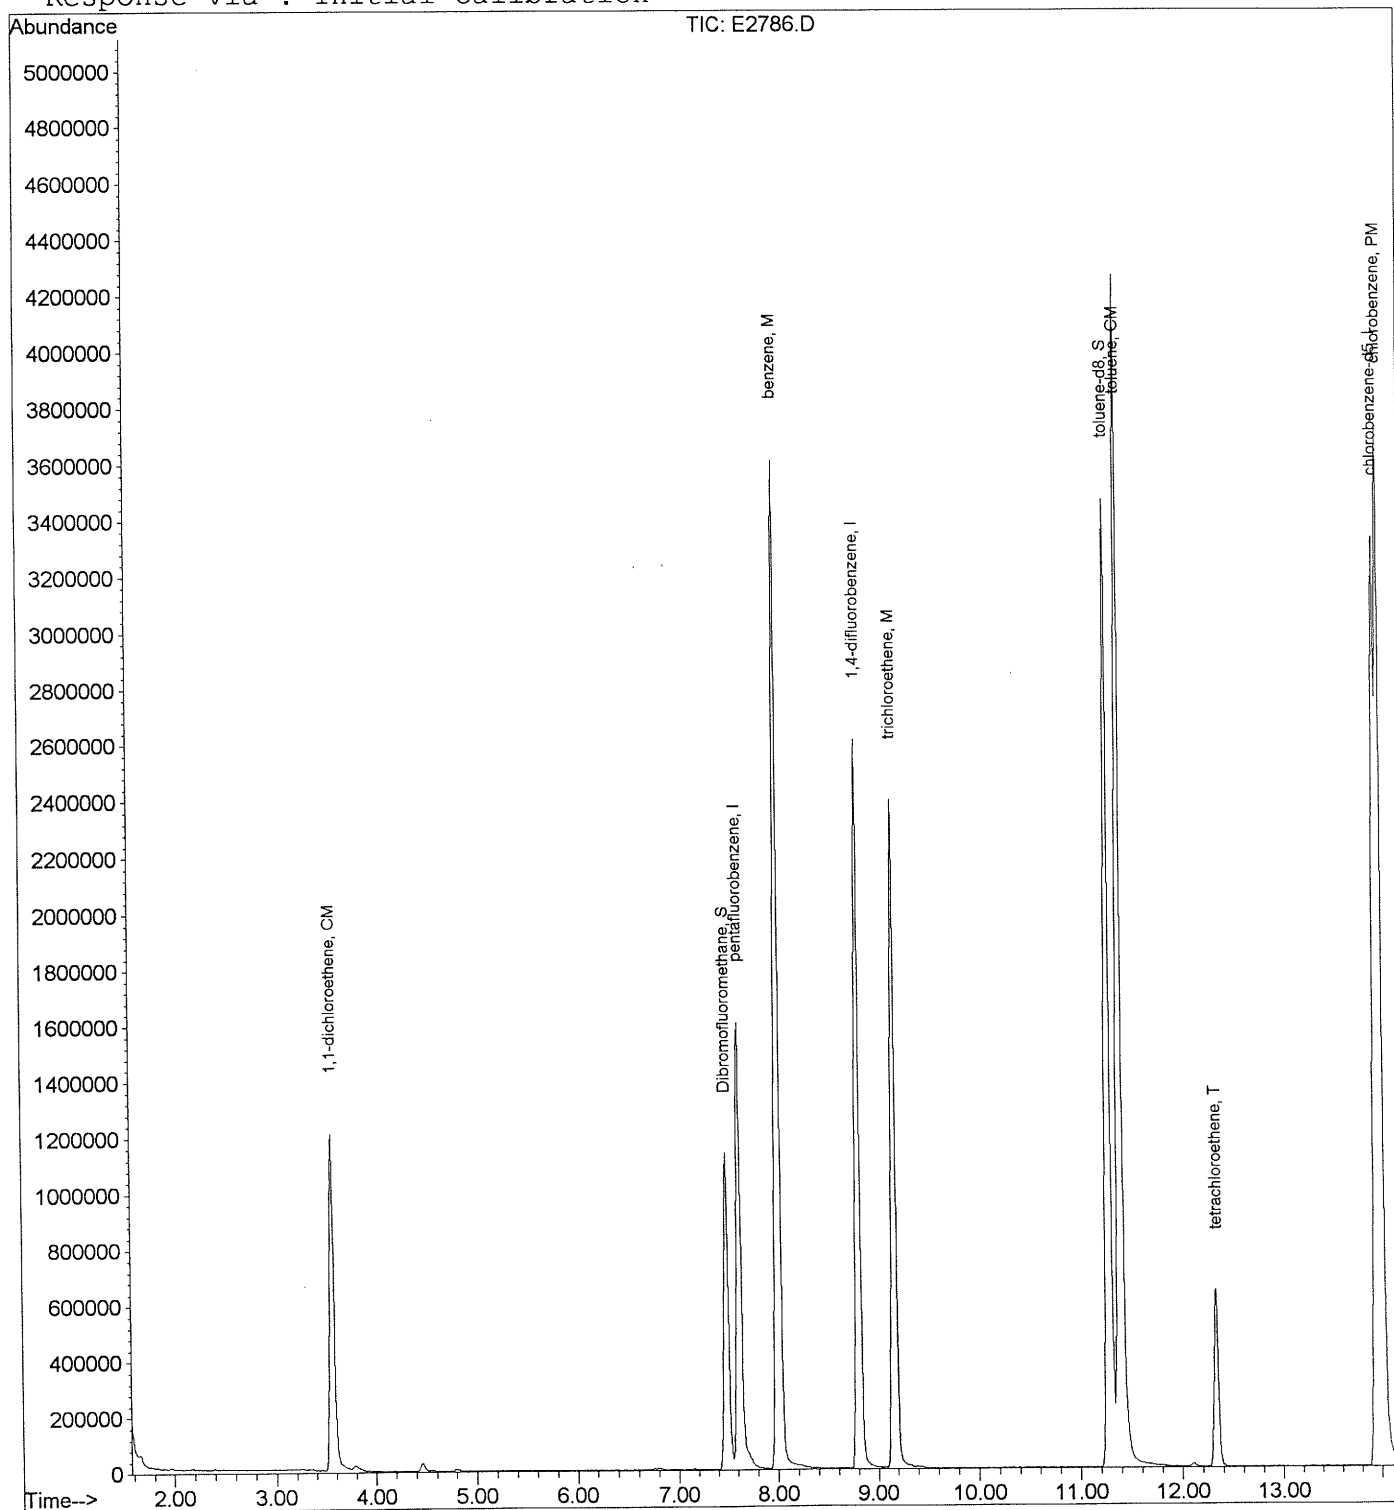


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2786.D
 Acq On : 29 Apr 05 4:04 pm
 Sample : 0504209-04amsd
 Misc : msd asp_8260s
 MS Integration Params: rteint.p
 Quant Time: May 2 6:35 19105

Vial: 13
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

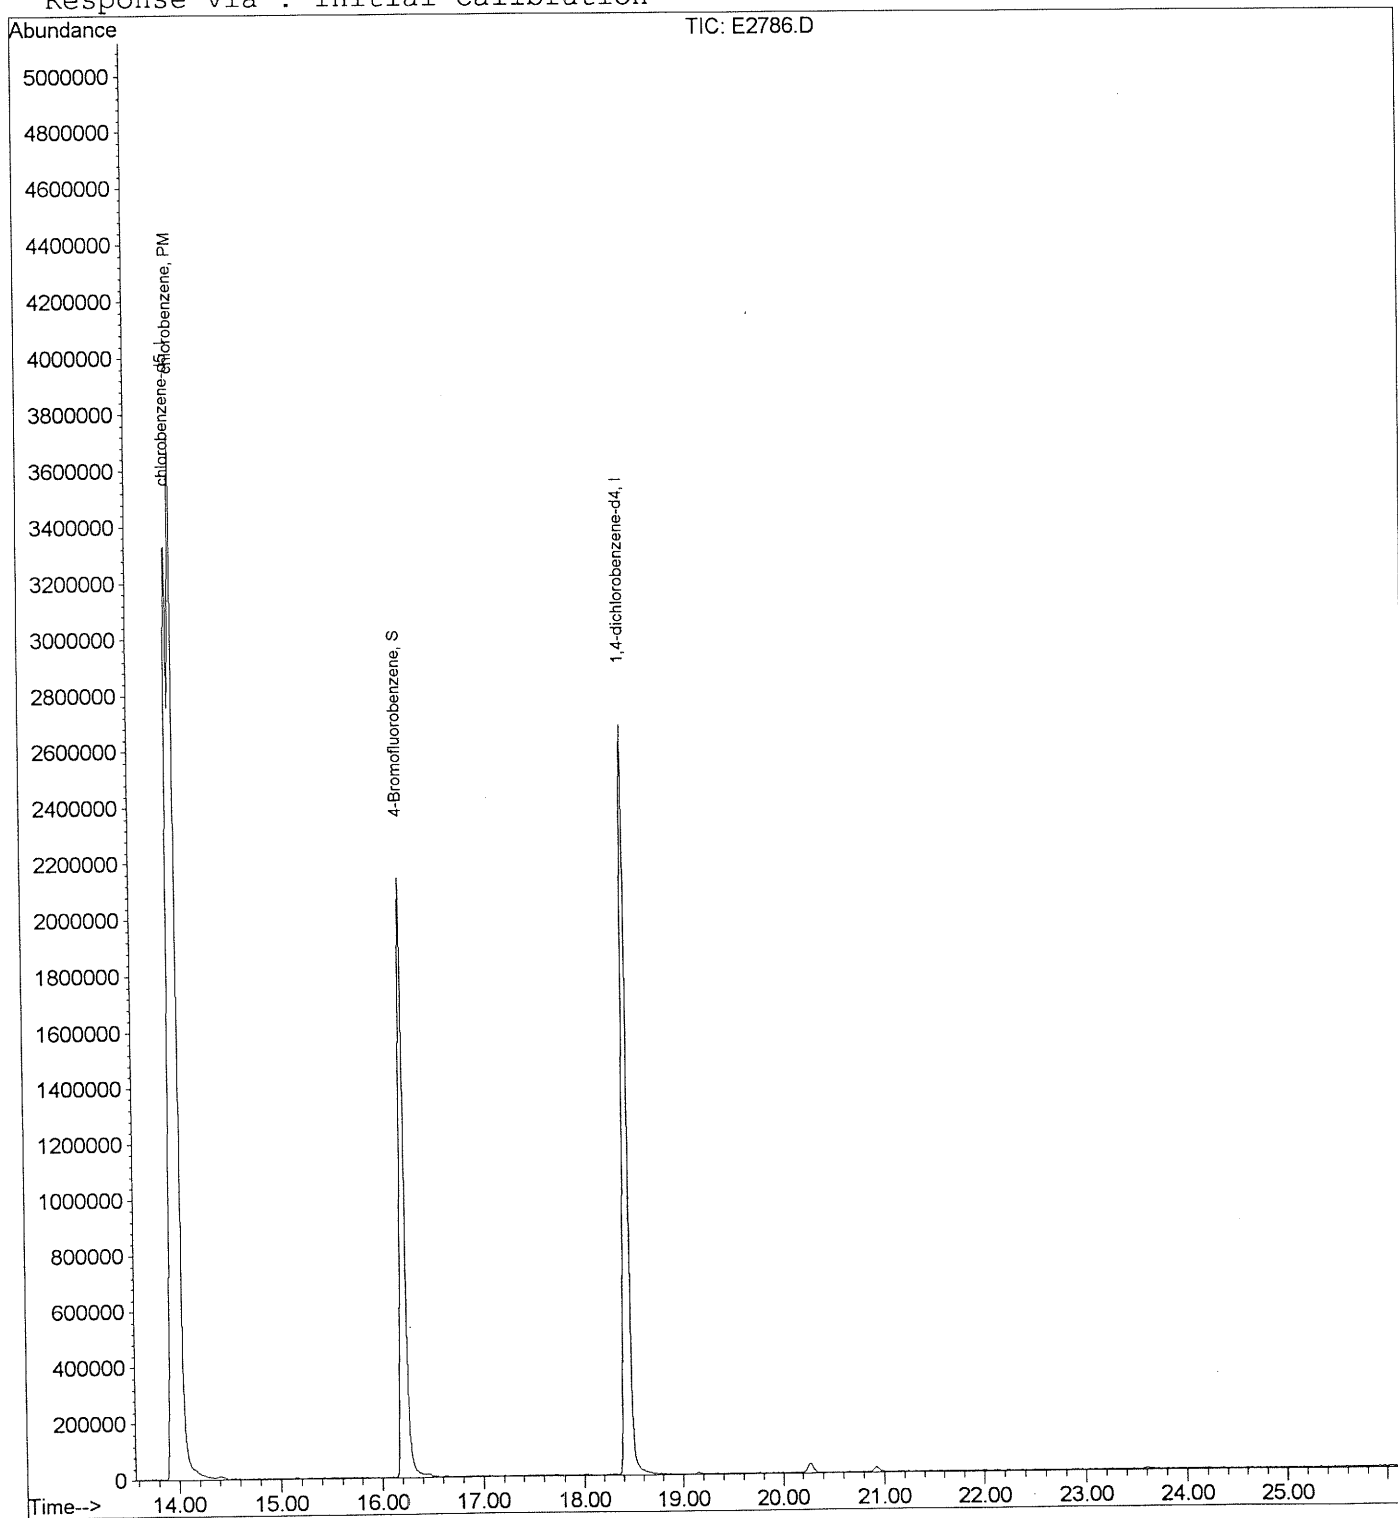

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 1cs042905

Sample wt/vol: 5 (g/mL) G Lab File ID: E2779.D

Level: (low/med) LOW Date Received: _____

% Moisture: not dec. Date Analyzed: 4/29/2005

GC Column: RTX-624 ID: 0.32 (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
630-20-6	1,1,1,2-Tetrachloroethane	54.6		D
71-55-6	1,1,1-Trichloroethane	55.4		D
79-34-5	1,1,2,2-Tetrachloroethane	43.2		D
79-00-5	1,1,2-Trichloroethane	48.1		D
75-34-3	1,1-Dichloroethane	51.9		D
75-35-4	1,1-Dichloroethene	61.2		D
563-58-6	1,1-Dichloropropene	53.8		DB
87-61-6	1,2,3-Trichlorobenzene	51.9		D
96-18-4	1,2,3-Trichloropropane	44.2		D
120-82-1	1,2,4-Trichlorobenzene	57.6		D
95-63-6	1,2,4-Trimethylbenzene	53.4		D
96-12-8	1,2-Dibromo-3-chloropropane	41.1		D
106-93-4	1,2-Dibromoethane	48.0		D
95-50-1	1,2-Dichlorobenzene	50.8		D
107-06-2	1,2-Dichloroethane	50.5		D
78-87-5	1,2-Dichloropropane	50.0		D
108-67-8	1,3,5-Trimethylbenzene	54.5		D
541-73-1	1,3-Dichlorobenzene	53.5		D
142-28-9	1,3-Dichloropropane	48.1		D
106-46-7	1,4-Dichlorobenzene	52.7		D
590-20-7	2,2-Dichloropropane	58.6		D
78-93-3	2-Butanone	37.5		D
110-75-8	2-Chloroethyl vinyl ether	386		DE
95-49-8	2-Chlorotoluene	49.4		D
591-78-6	2-Hexanone	42.8		D
106-43-4	4-Chlorotoluene	52.2		D
99-87-6	4-Isopropyltoluene	55.1		D
108-10-1	4-Methyl-2-pentanone	40.4		D
67-64-1	Acetone	40.6		D
107-13-1	Acrylonitrile	36		DJ
71-43-2	Benzene	54.0		D
108-86-1	Bromobenzene	51.7		D
74-97-5	Bromochloromethane	52.3		D
75-27-4	Bromodichloromethane	52.6		D
75-25-2	Bromoform	51.1		D

Lab Name: Toxikon Corporation Contract: _____

Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209

Matrix: (soil/water) Soil Lab Sample ID: 1cs042905

Sample wt/vol: 5 (g/mL) G Lab File ID: E2779.D

Level: (low/med) LOW Date Received: _____

% Moisture: not dec. Date Analyzed: 4/29/2005

GC Column: RTX-624 ID: 0.32 (mm) Dilution Factor: 1.00

Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane	79.6		D
75-15-0	Carbon disulfide	50.4		D
56-23-5	Carbon tetrachloride	56.3		DB
108-90-7	Chlorobenzene	52.1		D
75-00-3	Chloroethane	54.8		D
67-66-3	Chloroform	53.3		D
74-87-3	Chloromethane	47.1		D
156-59-2	cis-1,2-Dichloroethene	51.7		D
10061-01-5	cis-1,3-Dichloropropene	54.3		D
124-48-1	Dibromochloromethane	52.2		D
74-95-3	Dibromomethane	49.8		D
75-71-8	Dichlorodifluoromethane	53.7		D
100-41-4	Ethylbenzene	55.2		D
87-68-3	Hexachlorobutadiene	56.3		D
74-88-4	Iodomethane	79.6		D
98-82-8	Isopropylbenzene	53.4		D
1634-04-4	Methyl tert-butyl-ether	45.2		D
75-09-2	Methylene chloride	49.1		D
104-51-8	n-Butylbenzene	55.8		D
103-65-1	n-Propylbenzene	54.4		D
91-20-3	Naphthalene	47.3		D
135-98-8	sec-Butylbenzene	53.5		D
100-42-5	Styrene	54.0		D
98-06-6	tert-Butylbenzene	51.5		D
127-18-4	Tetrachloroethene	58.6		D
109-99-9	Tetrahydrofuran	35.5		D
108-88-3	Toluene	54.0		D
156-60-5	trans-1,2-Dichloroethene	54.5		D
10061-02-6	trans-1,3-Dichloropropene	54.4		D
79-01-6	Trichloroethene	53.8		DB
75-69-4	Trichlorofluoromethane	58.0		D
108-05-4	Vinyl acetate	48.2		D
75-01-4	Vinyl chloride	50.4		D
1330-20-7	Xylenes, Total	161		D



Lab Name: Toxikon Corporation Contract: _____
 Lab Code: 10778 Case No.: LBG WHIT SAS No.: _____ SDG No.: 0504209
 Matrix: (soil/water) Soil Lab Sample ID: lcs042905
 Sample wt/vol: _____ (g/mL) G Lab File ID: E2778.D
 Level: (low/med) LOW Date Received: _____
 % Moisture: not dec. Date Analyzed: 4/29/2005
 GC Column: _____ ID: _____ (mm) Dilution Factor: 1.00
 Extract Volume: _____ (µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
630-20-6	1,1,1,2-Tetrachloroethane	54.3		D
71-55-6	1,1,1-Trichloroethane	55.6		D
79-34-5	1,1,2,2-Tetrachloroethane	46.9		D
79-00-5	1,1,2-Trichloroethane	52.0		D
75-34-3	1,1-Dichloroethane	52.4		D
75-35-4	1,1-Dichloroethene	58.3		D
563-58-6	1,1-Dichloropropene	53.0		D
87-61-6	1,2,3-Trichlorobenzene	54.8		D
96-18-4	1,2,3-Trichloropropane	49.6		D
120-82-1	1,2,4-Trichlorobenzene	58.3		D
95-63-6	1,2,4-Trimethylbenzene	51.6		D
96-12-8	1,2-Dibromo-3-chloropropane	50.2		D
106-93-4	1,2-Dibromoethane	51.6		D
95-50-1	1,2-Dichlorobenzene	51.3		D
107-06-2	1,2-Dichloroethane	53.4		D
78-87-5	1,2-Dichloropropane	51.2		D
108-67-8	1,3,5-Trimethylbenzene	52.7		D
541-73-1	1,3-Dichlorobenzene	52.1		D
142-28-9	1,3-Dichloropropane	50.5		D
106-46-7	1,4-Dichlorobenzene	51.3		D
590-20-7	2,2-Dichloropropane	57.4		D
78-93-3	2-Butanone	45.7		D
110-75-8	2-Chloroethyl vinyl ether	69.6		D
95-49-8	2-Chlorotoluene	51.1		D
591-78-6	2-Hexanone	49.7		D
106-43-4	4-Chlorotoluene	50.4		D
99-87-6	4-Isopropyltoluene	53.0		D
108-10-1	4-Methyl-2-pentanone	48.0		D
67-64-1	Acetone	48.2		D
107-13-1	Acrylonitrile	45		DJ
71-43-2	Benzene	53.6		D
108-86-1	Bromobenzene	51.3		D
74-97-5	Bromochloromethane	53.9		D
75-27-4	Bromodichloromethane	53.8		D
75-25-2	Bromoform	55.6		D

Lab Name: Toxikon Corporation

Contract: _____

Lab Code: 10778

Case No.:

LBG WHIT

SAS No.:

SDG No.: 0504209

Matrix: (soil/water)

SoilLab Sample ID: lcs042905

Sample wt/vol:

(g/mL) GLab File ID: E2778.D

Level: (low/med)

LOW

Date Received:

% Moisture: not dec.

Date Analyzed: 4/29/2005

GC Column:

ID: (mm)

Dilution Factor: 1.00

Extract Volume:

(µl)

CONCENTRATION UNITS:

CAS NO.	COMPOUND	(ug/L or ug/Kg)	µg/Kg	Q
74-83-9	Bromomethane		52.0	D
75-15-0	Carbon disulfide		50.2	D
56-23-5	Carbon tetrachloride		55.8	D
108-90-7	Chlorobenzene		51.2	D
75-00-3	Chloroethane		54.3	D
67-66-3	Chloroform		54.3	D
74-87-3	Chloromethane		47.6	D
156-59-2	cis-1,2-Dichloroethene		53.7	D
10061-01-5	cis-1,3-Dichloropropene		55.9	D
124-48-1	Dibromochloromethane		54.0	D
74-95-3	Dibromomethane		53.7	D
75-71-8	Dichlorodifluoromethane		54.0	D
100-41-4	Ethylbenzene		53.6	D
87-68-3	Hexachlorobutadiene		57.4	D
74-88-4	Iodomethane		71.5	D
98-82-8	Isopropylbenzene		51.3	D
1634-04-4	Methyl tert-butyl-ether		48.3	D
75-09-2	Methylene chloride		50.2	D
104-51-8	n-Butylbenzene		53.8	D
103-65-1	n-Propylbenzene		51.8	D
91-20-3	Naphthalene		53.4	D
135-98-8	sec-Butylbenzene		51.4	D
100-42-5	Styrene		53.2	D
98-06-6	tert-Butylbenzene		50.2	D
127-18-4	Tetrachloroethene		56.4	D
109-99-9	Tetrahydrofuran		43.3	D
108-88-3	Toluene		53.8	D
156-60-5	trans-1,2-Dichloroethene		53.7	D
10061-02-6	trans-1,3-Dichloropropene		57.1	D
79-01-6	Trichloroethene		54.6	D
75-69-4	Trichlorofluoromethane		58.8	D
108-05-4	Vinyl acetate		51.2	D
75-01-4	Vinyl chloride		50.6	D
1330-20-7	Xylenes, Total		158	D

Data File : C:\HPCHEM\1\DATA\042905\E2778.D
 Acq On : 29 Apr 05 11:25 am
 Sample : lcs042905
 Misc : lcs asp_8260s
 MS Integration Params: rteint.p
 Quant Time: May 2 6:02 19105

Vial: 5
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration
 DataAcq Meth : 8260ES6

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) pentafluorobenzene	7.62	168	1858894	50.00	ug/Kg	0.01
32) 1,4-difluorobenzene	8.80	114	3399793	50.00	ug/Kg	0.01
49) chlorobenzene-d5	13.95	117	3352827	50.00	ug/Kg	0.02
63) 1,4-dichlorobenzene-d4	18.44	152	1630197	50.00	ug/Kg	0.02

System Monitoring Compounds

29) Dibromofluoromethane	7.48	113	1154237	49.74	ug/Kg	0.01
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.48%		
45) toluene-d8	11.27	98	3979833	50.04	ug/Kg	0.01
Spiked Amount 50.000	Range 81 - 120		Recovery =	100.08%		
62) 4-Bromofluorobenzene	16.21	95	1646797	50.94	ug/Kg	0.02
Spiked Amount 50.000	Range 74 - 121		Recovery =	101.88%		

Target Compounds

						Qvalue
2) dichlorodifluoromethane	1.68	85	1373283	53.98	ug/Kg	96
3) chloromethane	1.89	50	2284738	47.63	ug/Kg	98
4) vinyl chloride	2.01	62	1470090	50.62	ug/Kg	99
5) bromomethane	2.39	96	394950m	52.02	ug/Kg	99
6) chloroethane	2.53	64	791815	54.29	ug/Kg	100
7) trichlorofluoromethane	2.82	101	1564868	58.82	ug/Kg	97
8) Diethyl Ether	3.24	45	526728m	39.34	ug/Kg	94
9) Acrolein	4.81	56	355094m	234.85	ug/Kg	82
10) Acetone	3.78	43	454475	48.17	ug/Kg	99
12) 1,1-dichloroethene	3.56	96	892364m	58.33	ug/Kg	97
13) Iodomethane	3.80	142	361626	71.54	ug/Kg	96
14) methylene chloride	4.46	84	1458552	50.24	ug/Kg	98
15) Carbon Disulfide	3.84	76	4519369	50.16	ug/Kg	99
16) Acrylonitrile	5.01	53	381793	44.99	ug/Kg	98
17) tert-Butyl alcohol	4.76	59	1413943	435.58	ug/Kg	100
18) methyl tert-butyl ether	4.81	73	3142563	48.32	ug/Kg	100
19) trans-1,2-dichloroethene	4.83	96	1355785	53.69	ug/Kg	98
20) 1,1-dichloroethane	5.63	63	2546852	52.43	ug/Kg	97
21) di-isopropyl ether	5.65	45	4597529	47.44	ug/Kg	99
22) Vinyl Acetate	5.73	43	2246178	51.19	ug/Kg	98
23) ethyl tert-butyl ether	6.28	59	3691782	48.17	ug/Kg	98
24) 2-Butanone	6.74	43	727262	45.70	ug/Kg	100
25) 2,2-dichloropropane	6.55	77	1769586	57.37	ug/Kg	98
26) cis-1,2-dichloroethene	6.64	96	1555332	53.73	ug/Kg	99
27) bromochloromethane	7.04	128	740945	53.94	ug/Kg	98
28) chloroform	7.20	83	2644687	54.31	ug/Kg	99
30) Tetrahydrofuran	7.09	42	408189	43.32	ug/Kg	97

(#) = qualifier out of range (m) = manual integration

E2778.D 8260ES6.M Mon May 02 06:02:40 2005

Data File : C:\HPCHEM\1\DATA\042905\E2778.D

Vial: 5

Acq On : 29 Apr 05 11:25 am

Operator: xl

Sample : lcs042905

Inst : inst e

Misc : lcs asp_8260s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: May 2 6:02 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Apr 04 10:16:13 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) 1,1,1-trichloroethane	7.38	97	1917043	55.58	ug/Kg	98
33) carbon tetrachloride	7.60	117	1645912	55.78	ug/Kg	86
34) 1,1-dichloropropene	7.68	75	2183684	52.99	ug/Kg	99
35) benzene	8.01	78	5401705	53.58	ug/Kg	100
36) 1,2-dichloroethane	8.20	62	1921418	53.46	ug/Kg	100
37) tert amyl methyl ether	8.21	73	3076992	49.73	ug/Kg	99
38) trichloroethene	9.16	95	1532359	54.64	ug/Kg	97
39) 1,2-dichloropropane	9.62	63	1476190	51.24	ug/Kg	100
40) dibromomethane	9.84	93	977481	53.73	ug/Kg	94
41) bromodichloromethane	10.13	83	1936305	53.80	ug/Kg	99
42) 2-Chloroethyl vinyl ether	10.73	63	9464m	69.60	ug/Kg	100
43) 4-Methyl-2-Pentanone	11.22	43	1640042	47.96	ug/Kg	98
44) cis-1,3-dichloropropene	10.93	75	2228120	55.87	ug/Kg	100
46) toluene	11.39	92	3379865	53.78	ug/Kg	99
47) trans-1,3-dichloropropene	11.98	75	1985156	57.09	ug/Kg	99
48) 1,1,2-trichloroethane	12.30	83	1131103	52.02	ug/Kg	98
50) 2-Hexanone	12.73	43	1175859	49.74	ug/Kg	99
51) tetrachloroethene	12.33	166	1463759	56.42	ug/Kg	96
52) 1,3-dichloropropane	12.59	76	2232528	50.53	ug/Kg	99
53) dibromochloromethane	12.94	129	1459282	53.99	ug/Kg	96
54) 1,2-dibromoethane	13.13	107	1369788	51.58	ug/Kg	98
55) chlorobenzene	14.00	112	3690278	51.23	ug/Kg	99
56) 1,1,1,2-tetrachloroethane	14.19	131	1261059	54.33	ug/Kg	95
57) ethylbenzene	14.16	91	6546943	53.62	ug/Kg	100
58) m,p-xylene	14.40	106	4711220	105.24	ug/Kg	94
59) o-xylene	15.14	106	2284072	52.57	ug/Kg	96
60) styrene	15.20	104	4007184	53.22	ug/Kg	98
61) bromoform	15.59	173	945071	55.57	ug/Kg	95
64) isopropylbenzene	15.83	105	6395004	51.29	ug/Kg	100
65) bromobenzene	16.45	156	1560842	51.30	ug/Kg	98
66) 1,1,2,2-tetrachloroethane	16.60	83	1830634	46.86	ug/Kg	98
67) 1,2,3-trichloropropane	16.66	110	466226	49.60	ug/Kg	94
68) n-propylbenzene	16.62	91	7725228	51.83	ug/Kg	98
69) 2-chlorotoluene	16.82	91	4512892m	51.12	ug/Kg	99
70) 4-chlorotoluene	17.05	91	5103670	50.39	ug/Kg	98
71) 1,3,5-trimethylbenzene	16.98	105	5287588	52.69	ug/Kg	98
72) tert-butylbenzene	17.57	91	3074134	50.20	ug/Kg	100
73) 1,2,4-trimethylbenzene	17.71	105	5097069	51.60	ug/Kg	99
74) sec-butylbenzene	18.01	105	6586825	51.39	ug/Kg	99
75) 1,3-dichlorobenzene	18.29	146	2782436	52.12	ug/Kg	99
76) 4-isopropyltoluene	18.31	119	5237601	53.04	ug/Kg	98

(#)= qualifier out of range (m) = manual integration

E2778.D 8260ES6.M

Mon May 02 06:02:41 2005

Page 2

000170

Data File : C:\HPCHEM\1\DATA\042905\E2778.D

Vial: 5

Acq On : 29 Apr 05 11:25 am

Operator: xl

Sample : lcs042905

Inst : inst e

Misc : lcs asp_8260s

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: May 2 6:02 19105

Quant Results File: 8260ES6.RES

Quant Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)

Title : SW-846 Method 8260B

Last Update : Mon Apr 04 10:16:13 2005

Response via : Initial Calibration

DataAcq Meth : 8260ES6

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) 1,4-dichlorobenzene	18.49	146	2786516	51.31	ug/Kg	99
78) 1,2-dichlorobenzene	19.25	146	2677591	51.27	ug/Kg	99
79) n-butylbenzene	19.15	91	5024206	53.84	ug/Kg	99
80) 1,2-dibromo-3-chloropropan	21.20	75	277030	50.22	ug/Kg	95
81) 1,2,4-trichlorobenzene	23.04	180	1631351	58.32	ug/Kg	99
82) hexachlorobutadiene	23.33	225	805317	57.35	ug/Kg	98
83) naphthalene	23.58	128	4113916	53.44	ug/Kg	100
84) 1,2,3-trichlorobenzene	24.13	180	1555457	54.79	ug/Kg	96

xl 5/2/05


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2778.D
 Acq On : 29 Apr 05 11:25 am
 Sample : lcs042905
 Misc : lcs asp_8260s
 MS Integration Params: rteint.p
 Quant Time: May 2 6:02 19105

Vial: 5
 Operator: xl
 Inst : inst e
 Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
 Title : SW-846 Method 8260B
 Last Update : Mon Apr 04 10:16:13 2005
 Response via : Initial Calibration

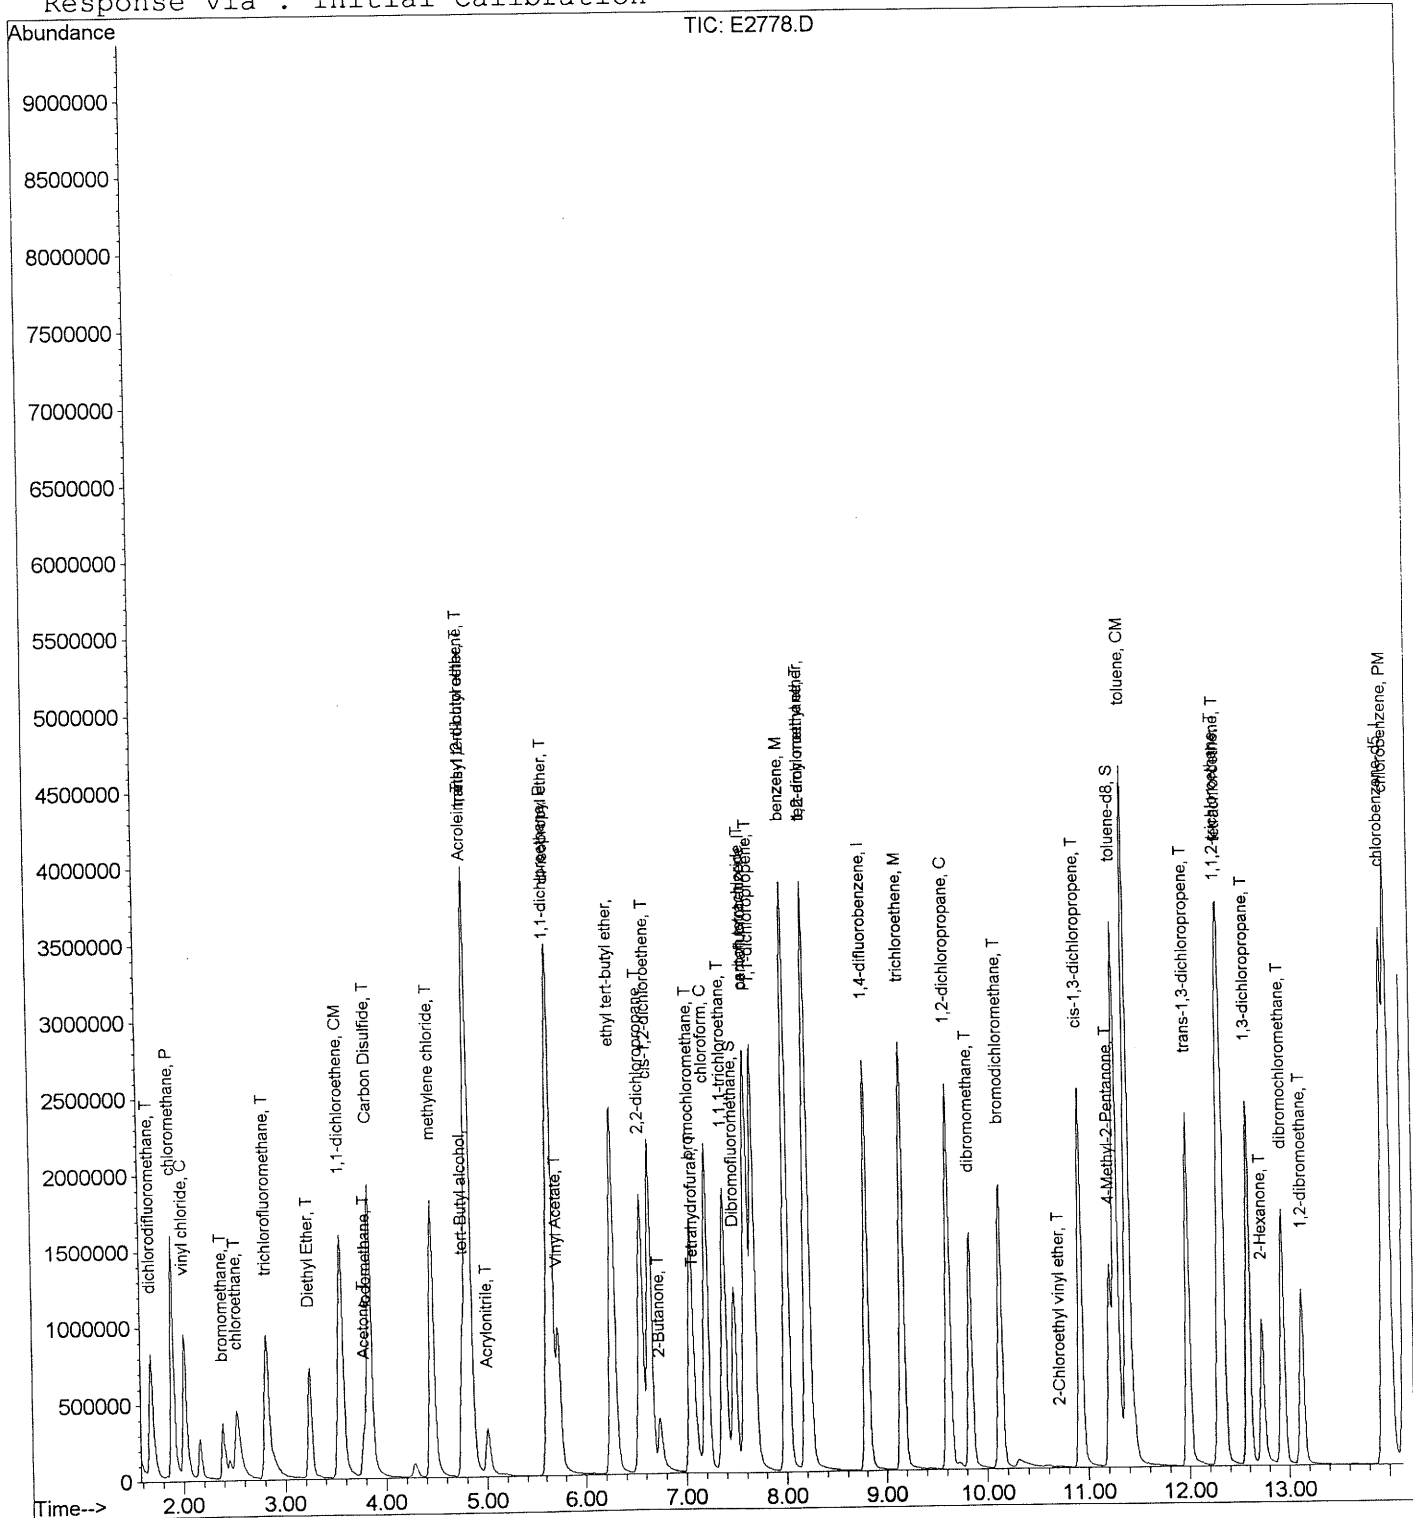


Quantitation Report

Data File : C:\HPCHEM\1\DATA\042905\E2778.D
Acq On : 29 Apr 05 11:25 am
Sample : lcs042905
Misc : lcs asp_8260s
MS Integration Params: rteint.p
Quant Time: May 2 6:02 19105

Vial: 5
Operator: xl
Inst : inst e
Multiplr: 1.00

Quant Results File: 8260ES6.RES

Method : C:\HPCHEM\1\DATA\042905\8260ES6.M (RTE Integrator)
Title : SW-846 Method 8260B
Last Update : Mon Apr 04 10:16:13 2005
Response via : Initial Calibration

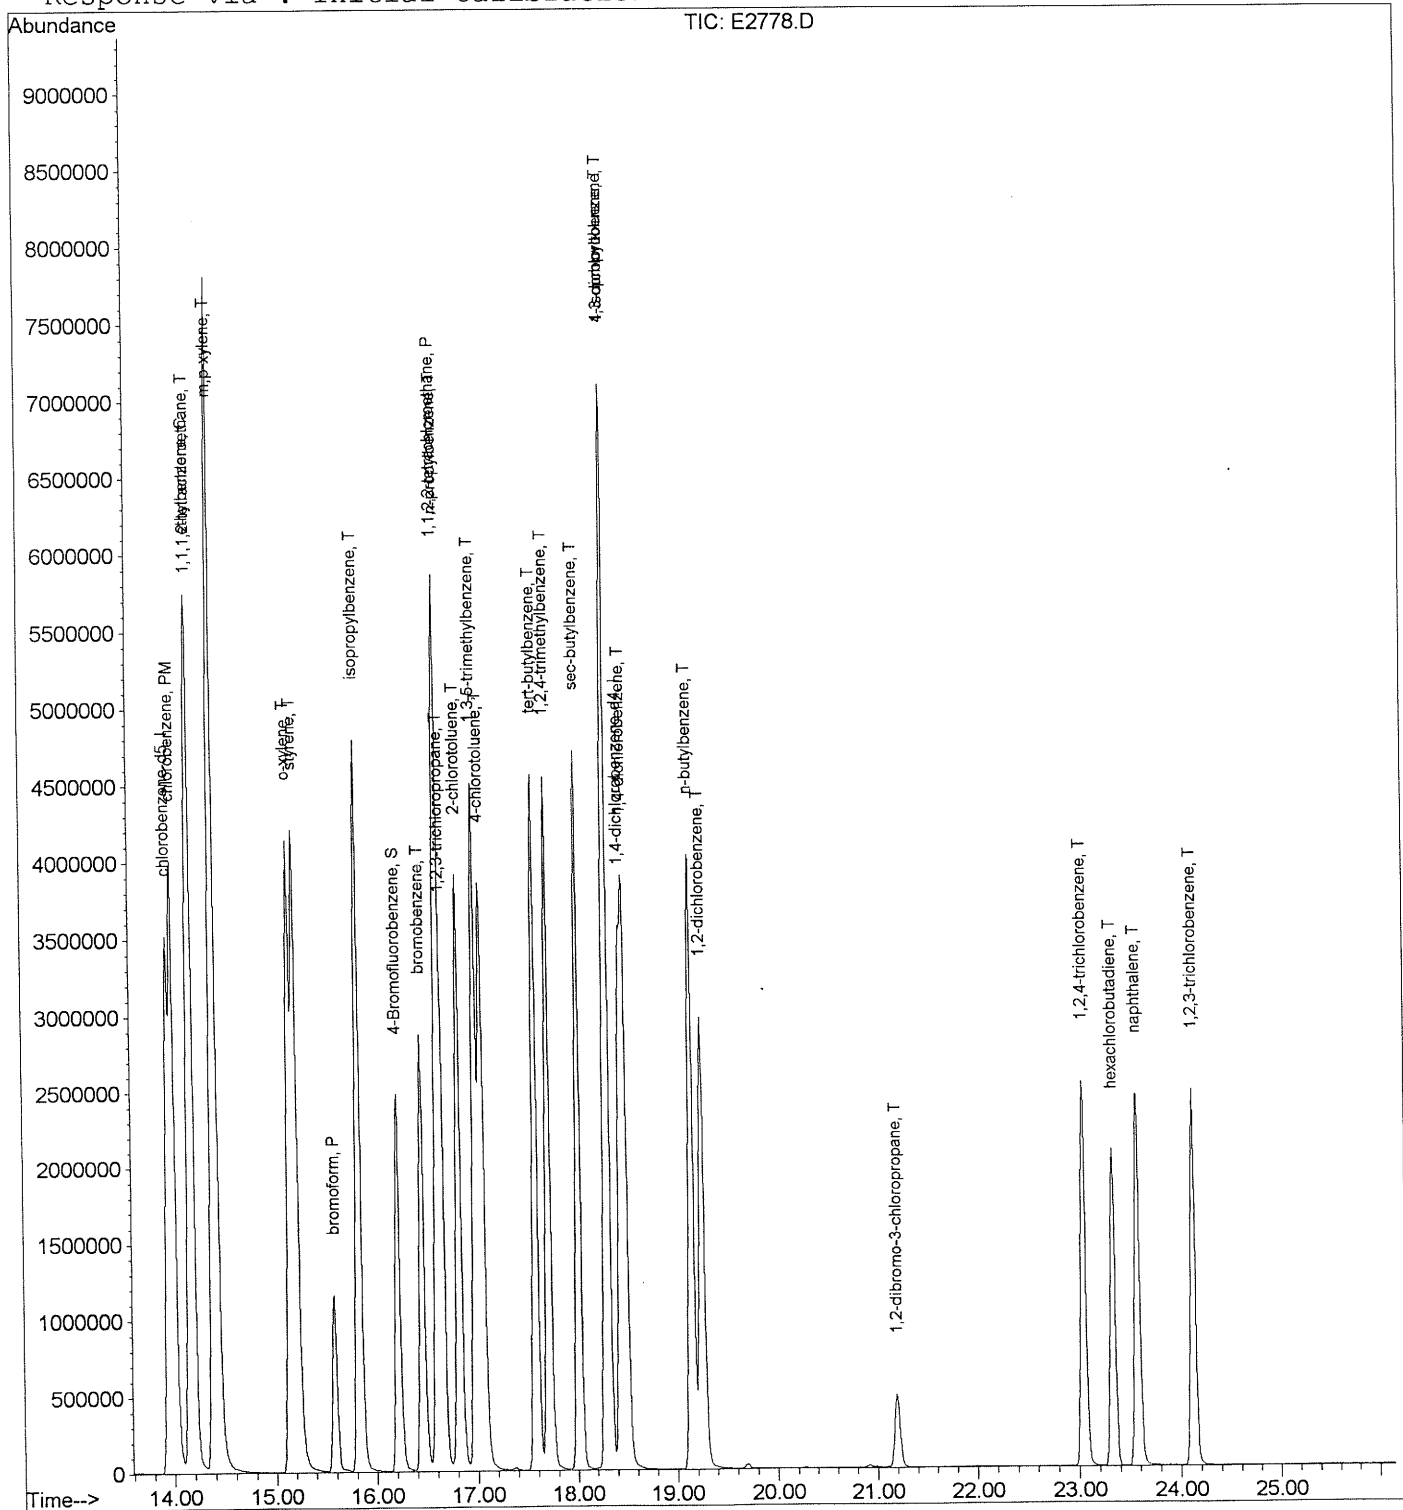

LOGBOOK PAGES

TOXIKON GC/MS VOLATILE ANALYSIS LOG INSTRUMENT E

MAINTENANCE PERFORMED:

WORKING STANDARD ID (enter when a new standard is used):

DATE	DATAFILE	CLIENT	LAB ID	SEQ	DILUTION	ALS	COMMENTS	OPERATOR
1 4/29/85	E2773		50mg RIBB			NI		XL
2	E2774		50mg RIBB STD			1	ABO.80105	XL
3	E2775		50mg RIBB STD			2		XL
4	E2776		50mg RIBB STD			3		XL
5	E2777		50mg RIBB STD			4		XL
6	E2778		50mg RIBB STD			5	SAVIL	XL
7	E2779		50mg RIBB STD			6	SAVIL	XL
8	E2780		50mg RIBB STD			7		XL
9	E2781		50mg RIBB STD			8		XL
10	E2782		50mg RIBB STD			9		XL
11	E2783		50mg RIBB STD			10		XL
12	E2784		50mg RIBB STD			11		XL
13	E2785		50mg RIBB STD			12		XL
14	E2786		50mg RIBB STD			13		XL
15	E2787		50mg RIBB STD			14		XL
16	E2788		50mg RIBB STD			15		XL
17	E2789		50mg RIBB STD			16		XL
18	E2790		50mg RIBB STD			17		XL
19	E2791		50mg RIBB STD			18		XL
20						19		XL
21						20		XL
22						21		XL
23						22		XL
24						23		XL
25						24		XL
26						25		XL
27						26		XL

000175

000114

%MOISTURE RAW DATA

Figure 1

DRY WEIGHT AND % MOISTURE DETERMINATION

Analyzed By/On: Am 4/26/05
Balance Used: OH405

[illegible]

Calc % Dry Weight: $[(\text{Gross Wt. Final-Tare})/(\text{Gross Wt. Initial-Tare})] \times 100 = \%$
 % Moisture is $100 - \% \text{ Dry Weight}$

Toxikon

Sample Receipt Checklist

Client L-B-G
Work Order Number: 05-04-209
Matrix 2/501L

Date and Time Received 4-27-05 10:00

Received by: SM

Reviewed by: _____

Initials

Date

Carrier name:

FEDEX

UPS

USPS

WALK-IN

COURIER

OTHER EAST

Shipping container/cooler in good condition?

Yes ☒

No ☐

Not Present ☐

Custody seals intact on shipping container/cooler?

Yes ☐

No ☐

Not Present ☒

Chain of custody present?

Yes ☒

No ☐

Chain of custody signed when relinquished and received

Yes ☒

No ☐

Chain of custody agrees with sample labels?

Yes ☒

No ☐

Samples in proper container/bottle

Yes ☒

No ☐

Sample containers intact?

Yes ☒

No ☐

Sufficient sample volume for indicated test?

Yes ☒

No ☐

All samples received within holding time?

Yes ☒

No ☐

Container/Temp Blank temperature in compliance?

Yes ☒

No ☐

N/A ☐

Water - VOA vials have zero headspace?

Yes ☐

No ☐

No VOA vials submitted ☒

Water- pH acceptable upon receipt?

Yes ☐

No ☐

N/A ☒

Checklist completed by: [Signature]

Signature

Date

Checked by: 4-27-05

Any No and/or NA (not applicable) response must be detailed in the comment section below.

Client contacted: _____ Date Contacted: _____ Person: _____

Contacted by: _____ Regarding: _____

Comments: _____

Corrective Action: _____

www.ecdelivers.com



(800) 877-4745

Guaranteed customized Express Parcel Service
from Maine to Virginia. Nationwide Same Day
Service. 365 Days a Year.

PACKAGE COPY

BOL# 20110359

Pick-Up Date	Pick-Up Time	Pick-Up Agent	Account #	Service Level	Route	Stop
4/20/01	12:44	273	10007 2	3	223	

2 FROM (Your Name)	Phone	3 TO (Recipient's Name)	Phone
MAINE C	(011) 666 5741	3	(811) 275-3330

Company	Exact Street Address	City	State	Zip Code	Room/Floor
TOXIKON	15 MIDDLE AVENUE	BEDFORD	MA	01730	

4 Shipper Billing Reference	Special Instructions

5 Release Signature	6 EC Guaranteed Express Parcel Services☆
	☐ Priority Letter (8 oz or less) - Delivery before 9 AM to major downtown business districts - 10:30 AM suburbs
	☐ Express Priority Overnight - Delivery before 9 AM to major downtown business districts - 10:30 AM suburbs
	☐ Next Business Day (By 5 pm)
	☐ Night Owl (Late Night Pick-up)
	☐ Same Day (Nationwide Next Flight or Door to Door Direct Drive)

By signing here, sender authorizes Eastern Connection to deliver this shipment without obtaining a delivery signature and shall hold harmless Eastern Connection from any claims resulting therefrom.

Pieces	Weight	Reweight
1	13 lbs.	
(Subject to correction)		

☐ Saturday Delivery (Not available to all Locations)	☐ Sunday/Holiday Delivery
☐ Early AM by _____ AM (Must call for prior arrangements)	



20110359